



norden

Nordic Innovation Centre

NT TECHNICAL REPORT

TR 569 Edition 3
Approved 2007-03

NORDTEST REPORT TR 569



Internal QUALITY CONTROL

Handbook for Chemical Laboratories

Authors: Håvard Hovind ¹⁾ Bertil Magnusson ²⁾ Mikael Krysell ³⁾ Ulla Lund ³⁾ Irma Mäkinen ⁴⁾	Nordic Innovation Centre project number: 04038	
	Institution: ¹⁾ NIVA, Norway ²⁾ SP Technical Research Institute of Sweden, Sweden ³⁾ Eurofins A/S, Denmark ⁴⁾ SYKE, Finland	
Title: Internal Quality Controll – Handbook for Chemical Laboratories		
Abstract: According to ISO/IEC 17025 (3): <i>The laboratory shall have quality control procedures for monitoring the validity of tests undertaken. The resulting data shall be recorded in such a way that trends are detectable and, where practicable, statistical techniques shall be applied to the reviewing of the results. The monitoring shall include e.g. regular use of internal quality control. ... Quality control data shall be analysed and, where they are found to be outside pre-defined criteria, planned action shall be taken to correct the problem and to prevent incorrect results from being reported.</i> Internal quality control at the chemical analytical laboratory, involves a continuous, critical evaluation of the laboratory's own analytical methods and working routines. The control encompasses the analytical process starting with the sample entering the laboratory and ending with the analytical report. The most important tool in this quality control is the use of control charts. The basis is that the laboratory runs control samples together with the routine samples. The results of the control program may be used in several ways - the analyst will have an important quality tool in his/her daily work, the customer can get an impression of the laboratory's quality and the laboratory can use the results in the estimation of the measurement uncertainty. The QC has to be part of a quality system and should be formally reviewed on a regular basis. The aim of this handbook is to describe a fit for purpose system for internal quality control at analytical laboratories that are performing chemical analysis. The approach is general, but the examples are mainly from environmental analyses.		
Technical Group: Environment		
ISSN: 0283-7234	Language: English	Pages: 46 p.
Key Words: Quality Control, Repeatability, Within Laboratory Reproducibility, Trollbook, Troll, X-chart, R-chart, Range, Uncertainty, Control limit, Warning limit, Action limit		
Distributed by: Nordic Innovation Centre Stensberggata 25 NO-0170 Oslo Norway	Report Internet address: info@nordicinnovation.net www.nordicinnovation.net	

Preface

The aim of the Troll book is to give good and practical guidance for internal quality control. It is written for **you** – working with routine determinations in the analytical laboratory.

The first version of *Internal Quality Control (1) – Handbook of Internal Quality Control in Water Laboratories* (Nordic cooperation) was prepared in 1984, and a revised version was printed in 1986 in Norway, best known under the name *Trollboken* (2). Later it has been translated to several other languages, and has been widely used as a tool in chemical routine laboratories – especially in environmental laboratories. This new version of the Handbook is an improved and extended edition, and the aim of it is – as has always been - that it should be a practical tool for the analysts in their daily work with the analytical methods.

During the years since the first version was prepared, there have been a lot of developments in the field of analytical quality. First of all the requirements for accreditation of analytical laboratories has put a pressure on the laboratories to document their analytical quality, and internal quality control is an important part of this documentation. When the first edition of accreditation standard was introduced, ISO/IEC 17025 (3), there was an increased focus on the concept of measurement uncertainty and traceability to a standard reference both in chemical and microbiological methods. When the laboratories estimate measurement uncertainty the results from internal quality control are essential. All these new demands have led to a need for a revision of the so-called *Troll book*.

The arrangement of the book has been changed to some extent, and in addition the chapters have been revised and updated. Several new practical examples have been worked out to demonstrate the applicability to different fields of chemical analyses.

The description of how to prepare calibration and QC solutions for water analysis is removed from the new version of the Troll book as the preparation of these solutions is properly described in the new ISO and CEN standards.

The task of compiling and editing this book has been made possible by the financial support from Nordic Innovation Centre/Nordtest through the project 04038, and also from the Swedish Environmental Protection Agency. The work would also have been impossible to perform without the effort of the Nordic working group consisting of:

Håvard Hovind, NIVA, Norway

Bertil Magnusson, SP, Sweden

Mikael Krysell and Ulla Lund, Eurofins A/S, Denmark

Irma Mäkinen, SYKE, Finland

For valuable comments on the contents we thank Håkan Marklund, Swedish Environmental Protection Agency, Annika Norling, SWEDAC, Roger Wellum, IRMM, and special thanks to Elisabeth Prichard, LGC, United Kingdom and Marina Patriarca and Antonio Menditto, ISS, Italy for their extensive comments. We also indebted to the many interested analytical chemists for their valuable suggestions. The working group also thanks Petter Wang, Norway, who made the Troll drawings to the original *Troll book*, and Timo Vänni, Finland, who prepared the new illustrations.

This handbook (version 3 of the new Trollbook about Internal Quality Control, 2007) can be downloaded from www.nordicinnovation.net technical report TR569

Information to our readers

The Trollbook starts, after an introduction, with two chapters (*Chapters 2 and 3*) on general issues of analytical quality, described with specific reference to internal quality control. They are followed by an introduction to internal quality control (*Chapter 4*).

The tools of control charting are described in the following chapters: control charts (*Chapter 5*), control samples (*Chapter 6*) and control limits (*Chapter 7*). *Chapter 8* summarises the tools in a description of how to start a quality control programme.

How the data of internal quality control are used is described in the following two chapters. *Chapter 9* explains the interpretation of quality control data to be performed after every analytical run, whereas *Chapter 10* explains how the quality control programme should be reviewed periodically to investigate if the programme is still optimal to control the quality of analyses.

Quality control data can be used for a number of purposes other than just control of the quality in every run. *Chapter 10* explains how information on the within-laboratory reproducibility, bias and repeatability is derived from quality control data, and *Chapter 11* gives examples of other uses of quality control data and the principles of control charting.

Chapters 12 and 13 give definitions and useful equations and tables for internal quality control and use of data from control charts.

Chapter 14 contains nine examples illustrating how control charts can be started as well as practical application of the control rules and the yearly review described in Chapters 9 and 10. In example 8 we present a detailed review of preliminary control limits and setting new control limits based on more data.

Chapter 15 lists references and suggested supplementary literature

Some common symbols and abbreviations used in this handbook are found below. Full explanation is given in Chapter 12.

s	Standard deviation
$\bar{x}$	Mean value
R_w	Within-laboratory reproducibility
CRM	Certified Reference Material
AL	Action Limit
WL	Warning Limit
CL	Central line
QC	Quality Control

CONTENTS

Preface.....	i
Information to our readers.....	ii
1. Introduction	1
2. Measurement uncertainty and within-laboratory reproducibility	3
3. Requirement for analytical quality.....	9
4. Principles of quality control charting.....	11
5. Different types of control charts	13
6. Different control samples.....	15
7. Setting the control limits	17
8. Setting up a quality control program.....	21
9. Daily interpretation of quality control.....	23
10. Long-term evaluation of quality control data.....	25
11. Other uses of quality control data and control charts.....	27
12. Terminology and Equations	29
13. Tables	33
14. Examples	35
15. References	46

1. Introduction

According to ISO/IEC 17025 (3): *The laboratory shall have quality control procedures for monitoring the validity of tests undertaken. The resulting data shall be recorded in such a way that trends are detectable and, where practicable, statistical techniques shall be applied to the reviewing of the results. The monitoring shall include e.g. regular use of internal quality control. ... Quality control data shall be analysed and, where they are found to be outside pre-defined criteria, planned action shall be taken to correct the problem and to prevent incorrect results from being reported.*

Internal quality control at the chemical analytical laboratory, involves a continuous, critical evaluation of the laboratory's own analytical methods and working routines. The control encompasses the analytical process starting with the sample entering the laboratory and ending with the analytical report. The most important tool in this quality control is the use of control charts. The basis is that the laboratory runs control samples together with the routine samples. The control values are plotted in a control chart. In this way it is possible to demonstrate that the measurement procedure performs within given limits. If the control value is outside the limits, no analytical results are reported and remedial actions have to be taken to identify the sources of error, and to remove such errors. Figure 1 illustrates the most common type of control chart, the X-chart.

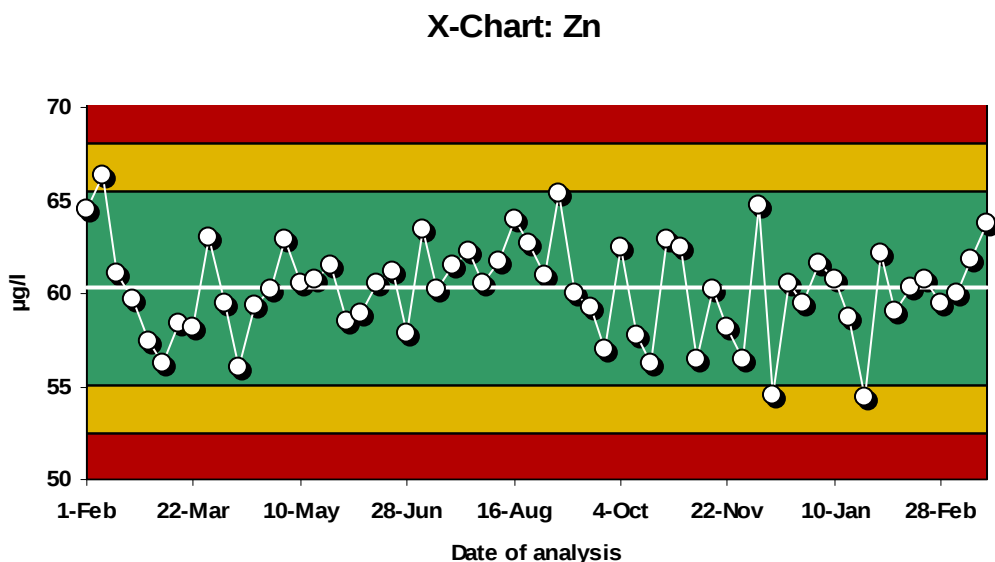


Figure 1. Example of an X control chart for the direct determination of zinc in water. All control values in the green area (within the warning limits) show that the determination of zinc performs within given limits and the routine sample results are reported. Control values in the red area (outside the action limits) show clearly that there is something wrong and no routine sample results are reported. A control value in the yellow area is evaluated according to specific rules.

When a quality control (QC) program is established, it is essential to have in mind the **requirement** on the analytical results and for what purposes the analytical results are produced – the concept of *fit for purpose*. From the **requirement** on the analytical results the analyst sets up the control program:

- Type of QC sample
- Type of QC charts
- Control limits – warning and action limits
- Control frequency

When the control program encompasses the whole analytical process from the sample entering the laboratory to the analytical report the control results will demonstrate the *within-laboratory reproducibility*. The *within-laboratory reproducibility* will indicate the variation in the analytical results if the same sample is given to the laboratory at different times.

The results of the control program may be used in several ways - the analyst will have an important quality tool in his/her daily work, the customer can get an impression of the laboratory's quality and the laboratory can use the results in the estimation of the measurement uncertainty.

The QC has to be part of a quality system and should be formally reviewed on a regular basis. Other important elements of the quality system are the participation in interlaboratory comparisons (proficiency tests), the use of certified reference materials and method validation.

In practical work it is necessary that the quality control is limited to fulfilling the requirements on the analytical results – a good balance between control work and analyses of samples is essential. The aim of this handbook is to describe a *fit for purpose* system for internal quality control at analytical laboratories that are performing chemical analysis. The approach is general, but the examples are mainly from environmental analyses.

2. Measurement uncertainty and within-laboratory reproducibility

This chapter introduces the terminology used in quality of analyses and the statistical background for quality control.

Analytical chemists know that a laboratory needs to demonstrate the quality of the analytical results. Depending on the customer's requirements it is either the spread in the results (repeatability or reproducibility) or the *measurement uncertainty* that is the important quality parameter. The internal quality control will normally give an indication of the *within-laboratory reproducibility*, R_w . The *within-laboratory reproducibility* will tell the customer the possible variation in the analytical results if the same sample is given to the laboratory in January, July or December. The *measurement uncertainty* will tell the customer the possible maximum deviation for a single result¹ from a reference value or from the mean value of other competent laboratories analysing the same sample.

From the laboratory's point of view the possible deviation from a reference value for an analytical result may be described by the laboratory ladder (4), Figure 2.

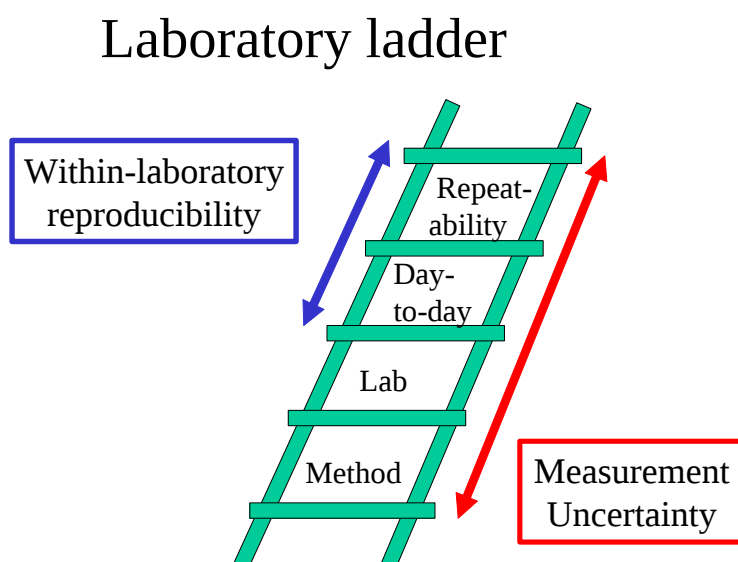


Figure 2. The ladder for a measurement procedure used in a laboratory

- Step 1 *The method bias – a systematic effect owing to the method used*
- Step 2 *The laboratory bias – a systematic effect (for an individual laboratory)*
- Step 3 *The day-to-day variation – a combination of random and systematic effects owing to, among other factors, time effects*
- Step 4 *The repeatability – a random effect occurring between replicate determinations performed within a short period of time; The sample inhomogeneity is part of the repeatability.*

¹ or more strictly the range of possible values with a defined probability associated with a single result

For an individual determination on a sample in a certain matrix the four different steps in the ladder are the following: 1) the method as such, 2) the method as it is used in the laboratory, 3) the day-to-day variation in the laboratory, 4) the repeatability of that sample. Each of these steps on the ladder adds its own uncertainty. The *within-laboratory reproducibility*, R_w , consists of step 3 and 4 - day-to-day variation and the repeatability. Repeated inter-laboratory comparisons will show the laboratory bias, step 2, and if different methods are used also the variation in method bias, step 1. The *measurement uncertainty* normally consists of all four steps.

Measurement uncertainty, as well as accuracy, is thus a combination of random and systematic effects. This is illustrated in Figure 3 where also different requirements on measurement uncertainty are illustrated with a small and a big green circle. For further reading about measurement uncertainty we recommend the Nordtest (5) and the Eurachem guide (6).

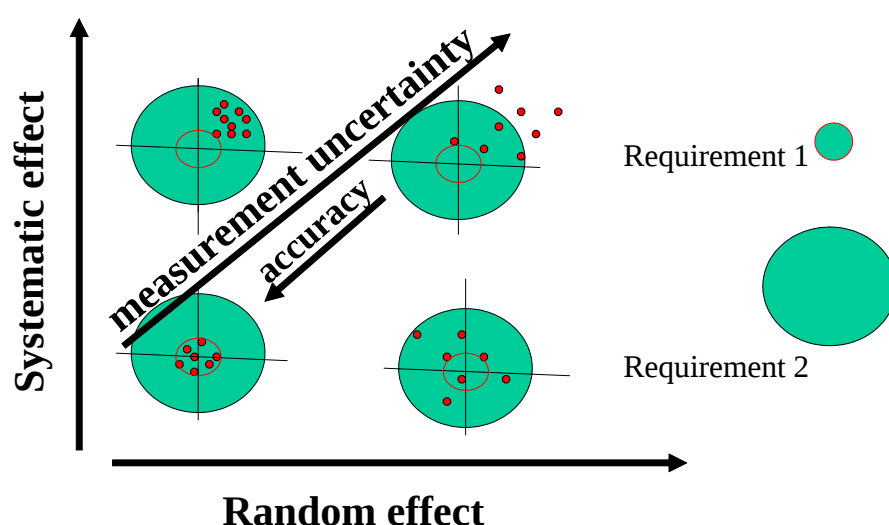


Figure 3. Random and systematic effects on analytical results and measurement uncertainty may be illustrated by the performance of someone practicing at a target – the reference value or true value. Each point represents a reported analytical result. The two circles are illustrating different requirements on analytical quality. In the lower left target requirement 1 is fulfilled and requirement 2 is fulfilled in all cases except the upper right. The upper left target represents a typical situation for most laboratories.

Repeatability and reproducibility

We use the notion *repeatability* when a sample (or identical samples) is analysed several times in short time (e.g the same day), by one person in one laboratory, and with the same instrument. The spread of the results under such conditions is representing the smallest spread that an analyst will obtain.

We use the notion *reproducibility* when a sample is analysed using the same analytical method under varying conditions, for instance when the analyses are performed at different times, by several persons, with different instruments, and in different laboratories.

The *within-laboratory reproducibility* (intermediate precision) will be somewhere in between these two outermost cases.

Bias

There is a bias when the results tend to be always greater or smaller than the reference value. Variations on bias may occur over a period of time because of changes in instrumental and laboratory conditions. For small changes it is often difficult to say if these effects are random or systematic.

Some typical sources of systematic effects (10):

- Instability of samples between sample collection and analysis
- Inability to determine all relevant forms of the analyte
- Interferences
A response for another substance in the matrix will also cause an effect of this type. If the slope of the calibration curve is different for calibration solutions and the natural samples there is also a systematic effect.
- Biased calibration
If samples and calibration standards are treated differently or if the matrix is different, this can represent a potentially serious source of error. Impurity of the material used to prepare calibration standards is, of course, another potential cause of systematic effect as well as if the calibration curve is supposed to be linear in a concentration range where this is not true.
- Blank correction too high or too low
If the blank and the sample are different and not treated in the same way.

Random variation and the normal distribution

Truly random variations from several sources added together can be described by a normal distribution. The irregular and uncontrollable variations in the many factors affecting the analytical result can be: small differences in the volume of reagents added, different reaction times, varying contamination from laboratory equipment and environment, instability in the instrument, uncertainty in the readings, temperature variations and different calibration solutions used etc.

Table 1. Example of laboratory internal quality control values for a solution containing 60,0 µg/l of zinc

64,5	66,3	61,1	59,7	57,4	56,2	58,4	58,2	63,0	59,5
56,0	59,4	60,2	62,9	60,5	60,8	61,5	58,5	58,9	60,5
61,2	57,8	63,4	60,2	61,5	62,3	60,5	61,7	64,0	62,7
61,0	65,4	60,0	59,2	57,0	62,5	57,7	56,2	62,9	62,5
56,5	60,2	58,2	56,5	64,7	54,5	60,5	59,5	61,6	60,8
58,7	54,4	62,2	59,0	60,3	60,8	59,5	60,0	61,8	63,8

If we analyse a sample several times, we do not obtain a series of identical results. The values are more or less spread within certain limits. The results are varying randomly, and we are not able to predict in which direction, and by how much. How may we describe the distribution of the results, and achieve a measure for the random variation? By visual evaluation of the control values in *Table 1*, we can hardly form a distinct picture of the analytical variation.

A graphical presentation of the results gives a much better understanding of the spread. Figure 4 is a histogram where the control values are collected into groups according to their concentration. Each group is represented by a column, the height of which is a measure of how many results this group consists of.

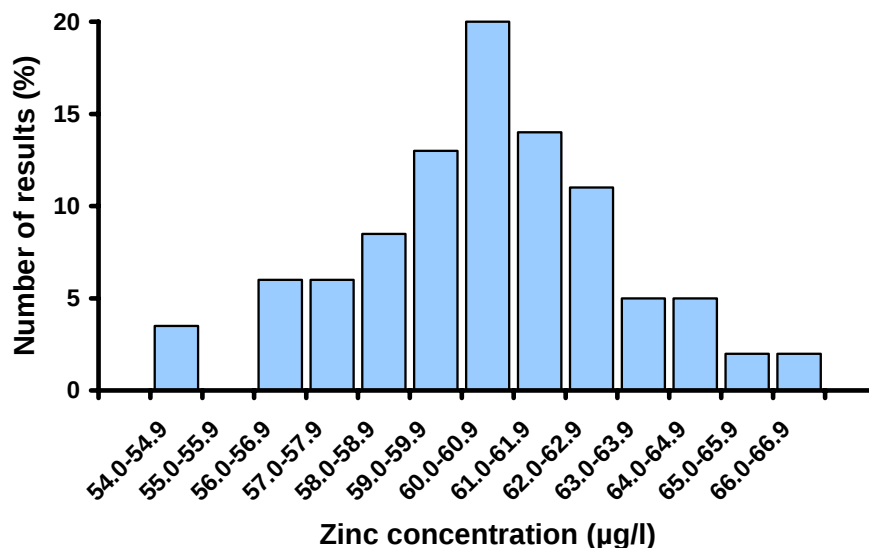


Figure 4. A histogram illustrating the distribution of the control values from the table given above. The results are sorted in groups defined by the concentration range. Each group is represented by a column where the height is representing the number of results in the group, calculated in percent of the total number of results.

If we increase the number of measurements, and collect the values in groups with increasingly narrower columns we will approach the smooth curve in Figure 5. This is an example of a frequency curve, the so-called normal distribution curve, constituting the basis of the control charts being used in the internal quality control.

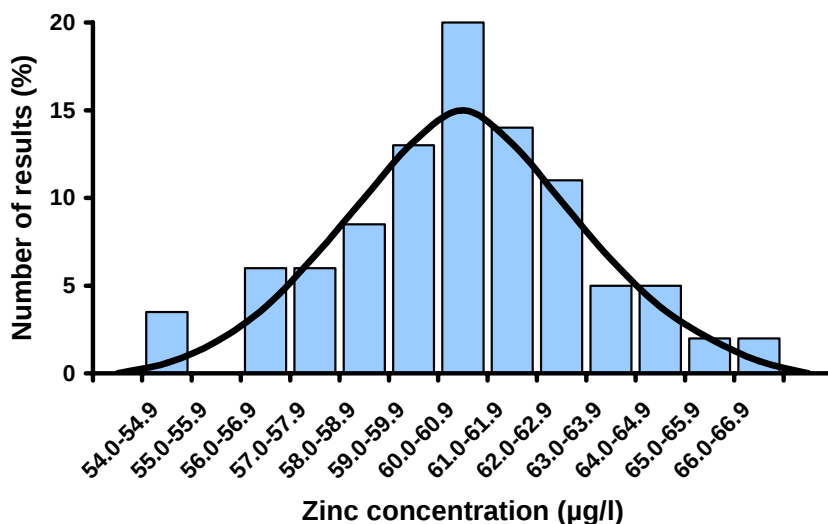


Figure 5. The relation between the normal distribution curve and the histogram. The distribution curve is based on the same data as represented in the histogram (Figure 4).

It is a presupposition to apply the statistical methods, based on the normal distribution curve, for the treatment of the control data. However, over a longer period in a laboratory the bias may vary with time, resulting in all control values being over (or under) the mean value for a time period. These results are out of statistical control, but may still be acceptable if the results are within the warning limits.

When the results are normally distributed, the mean value $\bar{x}$ is defined by the position of the maximum of the curve. The shape of the curve is determined by the spread of the single results, expressed by the standard deviation, s . This is illustrated in *Figure 6*.

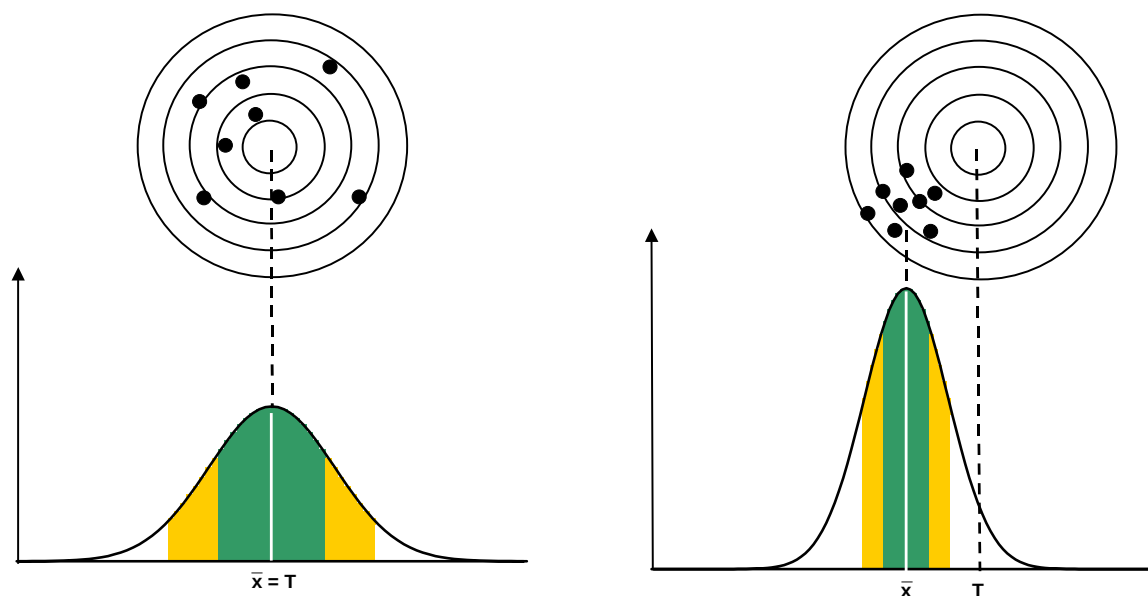


Figure 6. The shape of the normal distribution curve is depending on the spread in the analyses i.e.. within-laboratory reproducibility: A poor reproducibility will give a large standard deviation, and the corresponding curve is broad (left). If the reproducibility is good, the standard deviation is small and the normal distribution curve will be narrow (right). The position of maximum is demonstrating the trueness of the analysis: In the first example the mean value is coinciding with the true value. In the example to the right the results are systematically too low ($\bar{x}$ is the mean value, and T is the true value or reference value, bias is calculated as $\bar{x} - T$).

On the basis of the normal distribution we may calculate a theoretical spread of the results around the mean value, see *Figure 7*. About 95 % of all results will be located within the mean value $\pm$ two times the standard deviation, and 99.7 % of the results are located within $\pm$ three times the standard deviation. These properties are applied in the construction of the control charts.

When reporting within-laboratory reproducibility to a customer we will normally report it at the 95 % confidence level that is $\pm$ two times the standard deviation. This means that an average of about 19 results out of 20 will be within this range. The 95% confidence level is also often chosen when reporting an expanded measurement uncertainty to a customer and that will often be $\pm$ two times the combined standard uncertainty for chemical measurements.

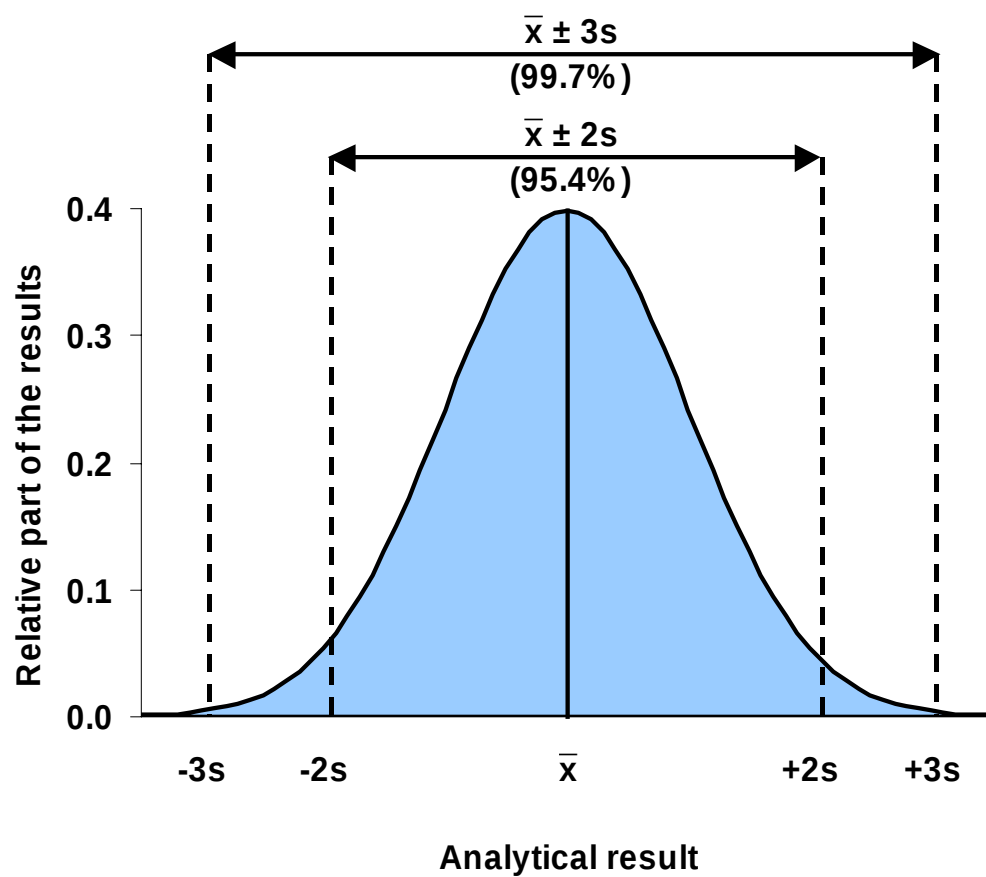


Figure 7. A normal distribution curve illustrating the probability for a result to be located within given limits ($\bar{x}$ is the mean value, s is the standard deviation).

3. Requirement for analytical quality

Here we describe how the analyst can translate the customer's requirement for quality into terms applicable to internal quality control, i.e. within-laboratory reproducibility (s_{RW}).

An analytical result can strictly speaking never be absolutely “correct”, since you will always get two slightly different results if you perform the same measurement twice. What *is* possible is to deliver a result with sufficiently small uncertainty for a given purpose, i.e. a result that is *fit for purpose*. Therefore we need to know the intended use of the result before we can define the requirements for quality.

Figure 3 in Chapter 2 illustrates that the quality sufficient for one purpose is not necessarily sufficient for all other purposes. It is also extremely important to remember that it is always the intended use of the data, not the capability of the laboratory that defines the necessary quality. Just as data can be too bad to be useful, it can also be too good, as too good often means too expensive or too slow to obtain!

An example: Analysis of wastewater discharge is normally done to monitor discharges so that legally allowable quality limits are not exceeded. These concentrations are relatively high compared to those in an unpolluted river or lake. Therefore the required limit of detection can be relatively high, but the measurement uncertainty must be adequate to ensure that the right decision is taken when comparing the result to the allowable concentration limit.



The users of the results expects to be able to trust the data, but in most cases they do not have the expert knowledge necessary to explain exactly what they need and they rely on the laboratory to supply the right answer to the problem – that is to deliver a result that is fit for the purpose. It is a challenge to the laboratory to understand the needs of the user. If the laboratory is accredited, the standard ISO/IEC 17025 requires that the laboratory evaluates the user's needs before any analyses are started.

Fortunately the majority of users for a specific parameter in a specific matrix, for example ammonium in drinking water, will need the analyses for the same purpose and therefore have the same requirements for quality. The laboratory therefore does not need to think closely on the subject every day but can design its quality control programme so that the data delivered will have the correct quality for the purpose.

But still the correct quality needs to be defined. In some cases national or regional authorities have defined the required quality for regulatory analyses. For example, the European drinking water directive 98/83/EC contains requirements for quality. If no such national or regional requirements for quality exist, the laboratory must prepare its own requirements, preferably in cooperation with the end-users of the results.

Experience has shown that uncertainty in most analytical systems is proportional to concentration until a limiting value is reached at low concentration where the uncertainty remains constant even though concentration in the sample decreases. Requirements for quality will therefore often consist of two sets of values, one given in concentration units (describing the limiting minimum uncertainty at low concentration) and one in percent (describing the proportional component of uncertainty at higher concentrations).

Requirements for the limiting minimum uncertainty are often described as a proportion (or percentage) of the concentration of primary interest. The “concentration of primary interest” may for example be a water quality limit or a similar allowable concentration.

The requirement for quality may be given as requirement for measurement uncertainty, but it is common to give the requirements using quality characteristics that can be measured directly, for example by internal quality control. For internal quality control the quality characteristic needed is *within-laboratory reproducibility*, s_{RW} . The example below shows how to start with uncertainty and from that estimate the demand for *within-laboratory reproducibility*.

Example:

Let us assume that we are asked to determine total nitrogen in wastewater and that the allowable limit for total nitrogen in the effluent you will analyse is 10 mg/l.

Our job as a laboratory is to ensure that the measurement uncertainty of our measurements is as low as we can reasonably make it for concentrations close to the limit value of 10 mg/l. A general recommendation in many EU directives is a s_{RW} of 5 % at that level².

Most laboratories will be able to determine total nitrogen with a relative s_{RW} of 5%. You will need to make sure that you give optimum quality at concentrations close to the limit value. A reasonable requirement would therefore be that you can analyse with a s_{RW} of 5% not only at 10 mg/l, but also at half that level, i.e. 5 mg/l. The required maximum s_{RW} measured in concentration units will therefore be 5% of $\frac{1}{2} \cdot 10 \text{ mg/l} = 0,25 \text{ mg/l}$.


The result is the following requirements for s_{RW} : 0,25 mg/l or 5%, whichever is higher. In practice this means that for all concentrations below 5 mg/l the required s_{RW} is 0,25 mg/l. From 5 mg/l and higher, the requirement is 5% s_{RW} .

² One example is the EU drinking water directive where a requirement of precision ($2 s_{RW}$) is 10 % of limit value for most parameters. The definition of precision in the directive is *Precision is the random error and is usually expressed as the standard deviation (within and between batch) of the spread of results about the mean. Acceptable precision is twice the relative standard deviation.*

4. Principles of quality control charting

This chapter describes the principles of quality control charts and what you do in the laboratory when running the samples, plotting and evaluating the results.

Control charting is a powerful and a simple tool for the daily quality control of routine analytical work. The basis is that the laboratory runs control samples together with the routine samples in an analytical run (Figure 8). Material of control samples can be standard solutions, real routine samples, blank samples, in-house control materials and certified reference materials.

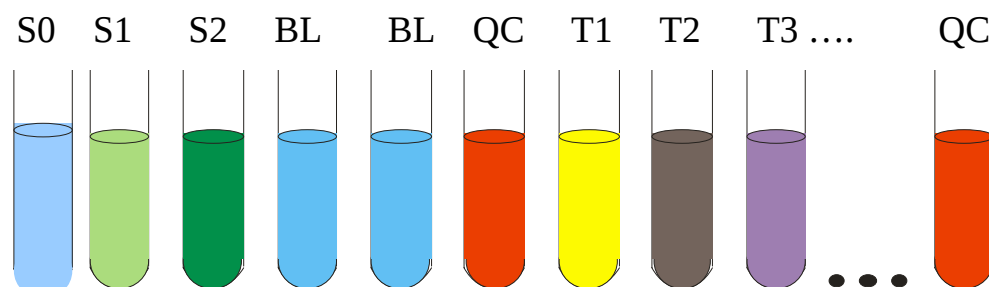

S0-S2 Standard solutions
BL Blank samples
QC Quality Control samples
T1... Test samples

Figure 8. Example of the analysis of two control samples in an analytical run.

Immediately after the analytical run is completed the *control values* are plotted on a control chart. When reporting the control values we recommend:

- giving one more significant digit compared to routine results.
- report **values** below reporting limit (LOQ)
- report negative **values**

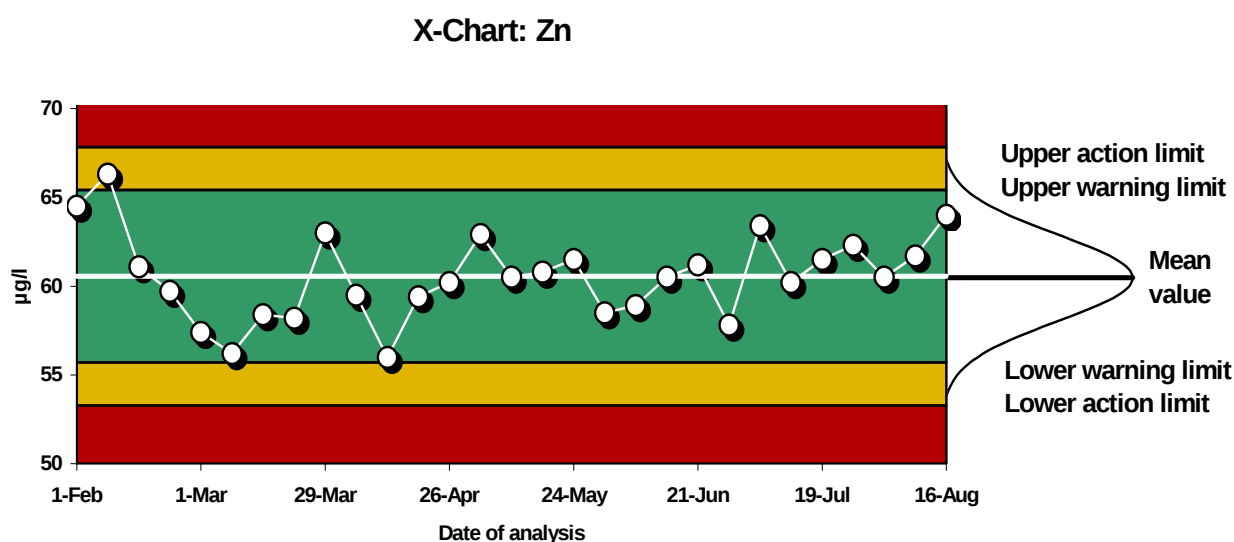



Figure 9. The relation between the normal distribution curve and the control chart.

The chart is based on the statistical characteristics of random variations, defined by the normal distribution curve. The relation between the normal distribution curve and the equivalent control chart (X-chart) is illustrated in *Figure 9*.

The central line (CL) in the control chart is representing the mean value of the control values or a certified value. In addition to the central line, the control chart normally has four lines. Two of these, the so-called *warning limits*, are located at a distance of $\pm$ two times the standard deviation from the central line ($CL \pm 2s$). Provided that the results are normally distributed, about 95 % of the results should be within these limits. In the control chart two other lines are also drawn at a distance of $\pm$ three times the standard deviation from the central line ($CL \pm 3s$). These lines are called the action limits and 99,7 % of the data normally distributed should be within these limits. Statistically only three out of 1000 measurements are thus located outside the action limits. If the control value is outside the action limits, there is a high probability that the analysis is in error.

The warning and action limits can be set either as above on method performance, *statistical control limits* or using independent quality criteria – *target control limits* – see Chapter 7.

Using the control charts, we should be alert if the control values are outside the warning limits or show trends. If values are outside the action limits no results are reported – see further Chapter 9.

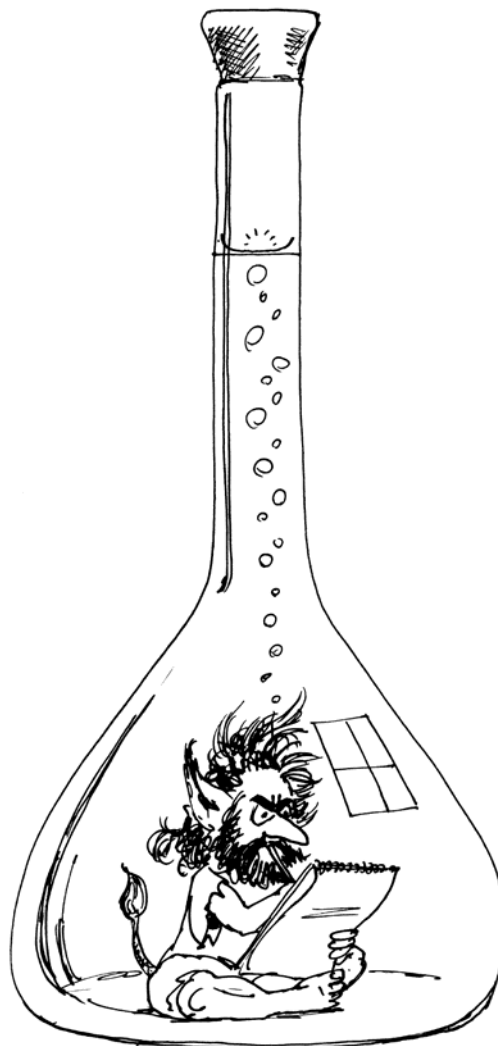

5. Different types of control charts

This chapter describes the different types control charts, when they will be used, and what they can be used for.

The following types of control charts are the most important ones used for the internal quality control of chemical analyses:

- X-charts
- Range-charts, R or r%

X-charts

An X-chart has a central line, upper and lower warning limits and upper and lower action limits.

One of the oldest and simplest types of control chart is the X-chart (7, 8, 9), which is based on the distribution of the control values around a true or expected value. It can be used to monitor the combination of systematic and random effects for control values, based on single results or on a mean of multiple analyses. Using a reference material similar to a routine sample as control sample, the bias may be monitored by comparing the mean control value over time with the reference value.

The *blank value chart* is a special application of the X chart, analyzing a sample that can be assumed to contain the analyte at a very low level. It provides special information about contamination of the reagents used, and the state of the measurement system. Even though concentrations are normally entered into the blank value chart, it is also possible to use the value of the measured signal. Remember that both positive and negative control values shall be plotted in the chart. In ideal cases the zero value should be the central line. However, the empirical mean value can be also used as the central line.

Another special case is a *recovery chart*. The analytical process may be tested for matrix influences by determining the recovery of spiked additions of standards to test samples. In this case a recovery rate of 100 % should be the central line.

Calibration parameters such as slope and intercept, in so far they are determined daily, can also be tested by means of the X chart.

Range charts

A range chart (R and r%) has a central line, an upper warning limit and an upper action limit. The X-chart shows how well control values (mean values of multiple analyses or single values) are within control limits. In contrast the range chart serves above all the purpose of repeatability control. The range is defined as the difference between the largest and smallest single result for two or more separate samples. For practical applications in analytical laboratories the R chart mostly appears only in its simplest form, only duplicate determination (of samples to be analysed) in each analysis series.

The best samples to be used are test samples selected among the samples to be analysed in that analytical run. However the concentrations may vary, because the samples are different in every analytical run. The range is normally proportional to sample concentration (at levels well above the detection limit) and then it will be more appropriate to use a control chart where the control value is the relative range r % (see Chapter 8).

If, for test samples, single determinations are made, the control value for the range chart should be based on the difference between single determinations of two (or more) different sample

aliquots. If on the other hand, test samples are run in duplicate we recommend that the control value is based on the mean value of duplicated determinations of two different sample aliquots – i.e. the same number of measurements for routine test samples as for control samples.



6. Different control samples

This chapter describes the most common types of control samples that can be used in quality control.

Ideally the control samples should go through the whole measurement procedure. They should also be very similar to test samples and stable over time. There should also be a sufficient amount for years and a suitable analyte concentration. This is however seldom the case and therefore we use several types of control samples:

- I Certified Reference Material – matrix CRM
- II Reference material, standard solution or in-house material
- III Blank sample
- IV Test (routine) sample

Control sample type I – certified reference material – matrix CRM

The results from repeated determinations of a matrix CRM will give a good indication of any systematic effect (bias). Repeated determinations in each analytical run give a possibility of using the standard deviation (or range) as an estimate of the repeatability of the measurement. However, when a CRM is used, there is generally a better repeatability compared to results obtained with a routine sample, due to better homogeneity.

A CRM is not always available for the desired sample matrix or concentration range. However, they are simple to use and the results give immediate information on both systematic and random effects. Furthermore, the results provide the laboratories with an opportunity to calculate their measurement uncertainty, and to compare their performance to that obtained by the certifying laboratories (see Chapter 11). Therefore, CRM's are recommended for use as often as practically and economically possible.

CRM's are purchased ready for use or with a procedure for preparation.

This control sample type is suitable for X-charts, and if multiple analyses are performed, also for R-charts.

Control sample type II – standard solutions, in-house or reference materials

Control sample type II may similarly to type I give an indication of some of the systematic effects as well as the random effects.

If the initial validation of the method has proved that the random effects, when analyzing control samples, are approximately the same as for test samples, this type of control will provide a direct measure for the within-laboratory reproducibility. However, in most cases the spread of the analytical results of a synthetic and a real sample will not be the same; therefore a stable real control sample should be chosen whenever possible.

A control sample type II is usually prepared by the laboratory. It can be either stable, homogeneous test samples or synthetic samples. Standard solutions can be bought from external suppliers but are often prepared in-house. For in-house matrix materials the laboratory collects the stable natural sample itself (or selects from samples received for analysis), making sure that the amount collected is sufficient to last for several years. Synthetic in-house materials are prepared from pure chemicals and purified solvent (e.g. water) simulating the matrix of test samples. Due care should be taken to prepare the control samples to get a stable level – we recommend that the uncertainty of the value of the analyte in the synthetic control sample should be less than one fifth of the standard deviation used to set up the control chart.

It is extremely important that chemicals used for preparation of synthetic materials are different from those used for calibration of the method. The difference can be either that the chemicals are purchased from different suppliers or for anions and cations that a different salt is used; for example for nitrate that a Na-salt is used for calibration and a K-salt for control. Most laboratories prepare stock control solutions that are diluted daily or at intervals, according to the laboratory's experience for stability of the diluted solution. If the same chemical, or worse, the same stock solution, is used for calibration and control, any error in preparation or purity of the chemical will not be seen.

This control sample type is suitable for X-charts, and if multiple analyses are performed, also for R-charts.

Control sample type III - blank sample

Control sample type III may be used for the surveillance of the limit of detection. Furthermore, this type of control sample serves to reveal contamination. Errors in the blank cause systematic effects at low concentrations, which can also be detected with control sample type III.

Control sample type III is the blank sample used for blank correction according to the procedure for analysis. No extra analyses are thus required to prepare a control chart for blank.

X-charts should be used, and R-charts can be used for this control sample type.

Control sample type IV test (routine) sample

Control sample type IV is used when the spread for control sample Type I or II is less than for test samples, for example if only synthetic materials or extremely homogenized CRM's are available. It is also valuable when it is not possible to have a stable control sample (type II) – typical examples are determination of dissolved oxygen and chlorophyll *a*. Duplicate measurements give a realistic picture of the within-run random variations for natural samples.

The control sample will generally be selected at random among the test materials submitted for measurement in the laboratory.

If a synthetic sample is used for the X-charts, it could be a good idea to include a control sample type IV, if the repeatability for synthetic and routine samples is different.

For this control sample type r%-charts are used. R-charts may also be used if the concentration of the test samples used as control samples is almost the same from day to day.



7. Setting the control limits

Here we present how to set the central line and set the control limits for X-charts and for R-charts.

Control limits may be set according to the performance of the analytical method used irrespectively of the requirement on analytical quality – *statistical control limits*. This is the most common method to set the limits. An alternative is to start with the analytical requirements or intended use of the results. From the requirement *within-laboratory reproducibility* is estimated and then the control limits are set – *target control limits*. In many cases it can be difficult to obtain specific requirements and then we recommend the use of *statistical control limits*.

Setting the control limits and the central line in X-chart

The control limits can be set based on method performance – **statistical control limits** or according to the requirement on *within-laboratory reproducibility* – **target control limits**.

Statistical control limits	Target control limits ³
The control limits are set based on the analytical performance of the control sample. From a longer time period, e.g. a year, the standard deviation s is calculated from the control values. Warning limits will be $+2 s$ and $-2 s$. Action limits will be $+3 s$ and $-3 s$.	The control limits are set based on the requirement on the analytical quality. The standard deviation for the control chart, s , is estimated from the requirement on s_{RW} Warning limits will be $+2 s$ and $-2 s$. Action limits will be $+3 s$ and $-3 s$.

The central line in the control chart can be the calculated mean value of the control values or a reference value for the control sample. In most cases a mean central line is used.

Mean central line	Reference central line
The mean value is estimated from control values obtained during a longer time, e.g. a year. The central line is set to this mean value.	The control sample is a reference material or a well-characterised material. The central line is set to the nominal value

In the cases below the control sample is an ideal control sample similar to routine samples and subjected to all steps of the analytical procedure and therefore the target s_{RW} may be used to set the target limits. The examples referred to below are presented in Chapter 14.

Case 1. **Statistical control limits** and a **mean central line** - see also Example 3 and Example 4
The requirement on *within-laboratory reproducibility* is not set and the method is performing with a $s_{RW} = 6 \%$. The warning limits are set to two times the method standard deviation, $\pm 12 \%$ and action limits to three times the standard deviation, $\pm 18 \%$. The mean value for the control sample is $59,2 \mu\text{g/l}$ so $\pm 12 \%$ is equal to $\pm 7,1 \mu\text{g/l}$ and $\pm 18 \%$ is equal to $\pm 10,7 \mu\text{g/l}$. The warning limits will be at $59,2 \pm 7,1 \mu\text{g/l}$ (52,1 and 66,3 $\mu\text{g/l}$) and the action limits will be at $59,2 \pm 10,7 \mu\text{g/l}$ (48,5 and 69,9 $\mu\text{g/l}$).

³ In the examples below we always assume that the number of samples analysed for control values is the same as used for routine measurements. If, however, a control value is based on duplicates (the mean of two response values) and a routine result is based on a single sample, and the major part of the spread is repeatability, the s used for setting the limits may have to be reduced.

Case 2. Statistical control limits and a reference central line.

If the mean value is very close to the nominal or the reference value, statistical control limits can be used otherwise we recommend case 4.

Case 3. Target control limits and a mean central line – see also Example 1 and Example 2.

The requirement on *within-laboratory reproducibility* is e.g. $s_{RW} = 5 \%$ and the method is performing with a lower s_{RW} . The warning limits are set to two times the standard deviation of the requirement, $\pm 10 \%$ and action limits to three times the standard deviation, $\pm 15 \%$. The mean value for the control sample is $59,2 \mu\text{g/l}$ so $\pm 10 \%$ is equal to $\pm 5,9 \mu\text{g/l}$ and $\pm 15 \%$ is equal to $\pm 8,9 \mu\text{g/l}$. The warning limits will be at $59,2 \pm 5,9 \mu\text{g/l}$ (53,3 and 65,1 $\mu\text{g/l}$) and the action limits will be at $59,2 \pm 8,9 \mu\text{g/l}$ (50,3 and 68,1 $\mu\text{g/l}$).

Case 4. Target control limits and a reference central line – see also Example 5 and Example 7.

The requirement on *within-laboratory reproducibility* is e.g. $s_{RW} = 5 \%$ and the method is performing with a lower s_{RW} . The warning limits are set to two times the standard deviation of the requirement, $\pm 10 \%$ and action limits to three times the standard deviation, $\pm 15 \%$. The mean value for the control sample is $59,2 \mu\text{g/l}$ but the reference value is $60,0 \mu\text{g/l}$ so the warning limits will be at $60,0 \pm 6,0 \mu\text{g/l}$ (54,0 and 66,0 $\mu\text{g/l}$) and the action limits will be at $60,0 \pm 9 \mu\text{g/l}$ (51,0 and 69,0 $\mu\text{g/l}$).

Setting the control limit in R-chart or r%-chart

For the range chart we only have upper limits – it is always positive. The control limits can be based on method performance – **statistical control limits** or according to the analytical requirement – **target control limits**. The statistical control limits are calculated from the measured mean range. The target control limits are calculated from a standard deviation, i.e. a target for repeatability (9). The factor used (2,83 & 3,69) for calculating the control limits can be found in Table 4 in Chapter 13 and also a background to these odd factors is explained in a comment to Table 4.

Statistical control limits	Target control limits
The control limits are set based on the analytical performance of the control sample. From a longer time period the mean range is calculated. For duplicate (n= 2) $s = \text{mean range}/1,128$. Central line is the mean range Upper warning limit will be + 2,83 s Upper action limits will be + 3,69 s	The control limits are set based on the requirement on repeatability. From the requirement a standard deviation s is estimated for this control chart. For n=2 Central line is 1,128 s Upper warning limit will be + 2,83 s Upper action limits will be + 3,69 s

Case 1. **Statistical control limits** – see also Example 3 (R) and Example 6 (r%) in Chapter 14. The mean range over a longer time period is 0,402 % (abs). The standard deviation is then $0,402/1,128 = 0,356$. The warning limit for the range chart will then be set at $+ 2,83 \cdot 0,356 = 1,0$ % and action limit $3,69 \cdot 0,356 = 1,3$ %.

Case 2. Target control limits.

The *repeatability limit*, r is often given in standard method and in this case as 1 % (in 19 times out of 20 the difference between two results should be less than 1 %). From this limit the repeatability standard deviations is calculated as $s_r = r/2,8^4 = 0,357$ %. The warning limit for the range chart will then be set at $+ 2,83 \cdot 0,357 = 1,0$ % and action limit $3,69 \cdot 0,357 = 1,3$ %.

⁴ The value 2.8 comes from error propagation of a difference where the repeatability limit is equal to $2 \cdot \sqrt{2} \cdot s$

Target control limits – estimating the s for the control sample

When the control sample encompasses the whole analytical process from the sample entering the laboratory to the analytical report the control values will demonstrate the *within-laboratory reproducibility*, s_{RW} , and one can compare the obtained s_{RW} with the requirement. With most other control samples, e.g. standard solutions, blank samples, the obtained standard deviation is just part of the s_{RW} . Here the analyst has to estimate if the obtained s on the control sample is sufficiently low to fulfil the analytical requirement - see Chapter 3.

Recommendations

Start of QC - In order to start the quality control of a new method preliminary control limits and central line can be estimated based on about 25 control values. Only after a longer time period, e.g. one year, can the control limits and the position of the central line be fixed. These first *preliminary* warning and action limits can also be based on results from method validation.

Fixed control limits – We do recommend fixed limits and not limits that are constantly changing for stable QC samples. In order to obtain reliable statistical control limits the calculated standard deviation should be based on control values over a one-year period and at least 60 control values. If the time period is shorter usually a too low estimation of the standard deviation is obtained since not all variation is taken into account.

Fixed central line – We recommend fixed central line. In order to obtain a reliable central line a one-year period may be a good time period. If the time period is shorter an unreliable estimate is easily obtained.

Replicate analyses/samples - We also recommend the same number of sub-samples being used both for routine samples and control samples – if we report the mean value of duplicates (e.g. the whole process) for test samples we should also in the X-chart plot the mean value of duplicate analyses for the control sample. If a control sample is analysed several times in the same run, either one or all control values can be plotted in the X-chart.

Multielement analyses – When many analytes are measured in the same analytical run in QC e.g. ICP, XRF, GC, we strongly recommend using target control limits or wider statistical limits for those analytes that are less important. If for example 20 analytes are determined⁵ and statistical control limits are used for all analytes, on average one control value (equal to 5 % of the control values) can be expected to be outside the warning limits in each analytical run. Also in about 1 out of 17 analytical runs a control value for one of the analytes is expected to be outside action limit, making ordinary interpretation very unpractical.

⁵ This applies to independent measurements and, to a lesser extent, also to measurements which are partially correlated such as ICP, XRF etc.

8. Setting up a quality control program

This chapter describes how to start setting up QC for a measurement procedure: selection of the number of control samples, the type of charts and the frequency of control analyses.

An example of setting up the QC (Cd determination in fresh waters)

Setting up the QC can best be described by a practical example: Cadmium concentration can normally vary between 0,01 µg/l and 100 µg/l in different types of waters. For quality control of Cd in fresh waters using ICP/MS (LOD 0,01 µg/l) we have chosen the control samples as follows:

Control samples	Control chart	Control limits	Central line
A CRM, Cd: 2,28 µg/l (Type I)	X-chart	Statistical	Reference value
A standard solution, Cd: 20 µg/l (Type II)	X-chart	Statistical	Mean value
An in-house material, Cd: 0,10 µg/l (Type II)	X-chart	Target	Mean value
Replicate determinations of test water samples in two concentration ranges, (Type IV)	r-% chart	Target	Target $s_r \cdot 1,128$



Because of the rather wide concentration range in routine samples we have chosen 3 QC samples Type I and II. The standard solution of 20 µg/l is prepared from a stock solution, which is not the same stock solution as used for the preparation of the calibration solutions. The in-house material, acidified lake water was prepared for quality control of low Cd content in fresh water.

For a direct check of systematic effects in our measurement procedure we use the CRM with a certified Cd content of $2,279 \pm 0,096$ µg/l.

In order to get a realistic picture of the repeatability for test samples we select at random two samples in each analytical run representing two concentration ranges and the these samples are analysed as duplicates (two different test tubes in the autosampler).

In measurement of Cd using ICP/MS we may carry out as many as 200 determinations in each analytical run. At the beginning and at the end of each run we analyse the CRM, the standard solution, the in-house material and the calibration standards. In order to check

calibration drift during a run, we normally analyse one of our control samples about every 20 analyses.

All the results obtained for the control samples are plotted in X-charts using our LIMS system. The results of duplicates obtained in analysis of routine test samples are plotted in r%-charts.

Practical points in setting up the QC

A method validation is normally performed before a measurement procedure is adopted. When setting up a programme for control charting, (such as selection of control samples, type of control charts and control frequency) the results of the initial tests for establishing performance of an analytical method may give valuable background information about e.g. the concentration range, the stability and systematic effects. In particular, a within-laboratory reproducibility of measurements in different concentrations obtained during a longer period in method validation forms the first basis for routine quality control.

Concentration range - In analysis of environmental samples concentrations of an analyte may vary considerably. In such cases it may be necessary to utilise separate X-charts and range charts for different concentration levels.

Range chart with test samples – To monitor repeatability using range charts (R-chart or r%-chart) we recommend analysing a test sample in duplicate in each analytical run. A test sample is selected at random and representative of the concentration range and matrix variations of the analyte being studied.

Frequency of control analyses - Generally, as a minimum, one control sample in each analytical run must be analysed for detecting possible systematic effects within the analytical run, for example from calibration. Stability of the measurement system can have an influence on the frequency of control analyses. If there are errors caused by calibration drift, the number of control samples to be analysed in each analytical run may need to be higher than under very stable measurement conditions. The principle guiding the decision on the number of times a control sample must be analysed in each analytical run is that all measurements performed after the last approved sample in the quality control may have to be reanalysed. The frequency of control is therefore a balance between the cost of the control and the cost of repeating analyses. When using automatic analysers, e.g. over night, several control samples may be analysed in each analytical run.

Position of control samples in an analytical run - The analyses of control samples should in principle be carried out in random order to eliminate any systematic effects. However, we recommend that control samples are analysed at least at the beginning of each run and before finishing the analytical run, in case a drift in the analytical process can cause errors.

A good balance between QC and test samples – QC fit for purpose. In this example we use several QC but in most cases fewer control samples will be sufficient.

QC program in a method description and in a quality manual

The principles of the quality control program covering the practical points mentioned above should be described in the quality manual of the laboratory. Quality procedures should also be presented in detail in the procedure of each analytical method.

First of all, the quality control measurements have to be fit for the purpose of the analyses.

9. Daily interpretation of quality control

In this chapter we describe the interpretation after each analytical run. Can we report the results or not? Is the method out of statistical control?



is out of statistical control

A practical procedure for the registration of the control data is to write down all information that may be significant for the interpretation of the control data. Typical examples are when new stock or control solutions have been prepared, e.g. the change of reagents, the change of measurement cell, and instrumental problems. If all information is properly documented it is, at a later time, possible to check the conditions for this determination e.g. in out of control situations.

For each batch of analyses there is normally one control value for each chart. In daily work it is essential to be alert if a control value is falling outside the control limits or if a certain systematic pattern is observed in the control values over a period of time.

Daily interpretation

There are three possible cases:

1. The method is in control
2. The method is in control but the long-term evaluation shows that the method
3. The method is out of control

1. The method is **in control** if:



- the control value is within the warning limits



- the control value is between warning and action limit and the two previous control values were within warning limits

In this case the analyst can report the analytical results.

2. The method is **in control** but can be regarded as **out of statistical control** if all the control values are within the warning limits (maximum one out of the last three between warning and action limit) and if:



- seven control values in consecutive order gradually increasing or decreasing (10)



- 10 out of 11 consecutive control values are lying on the same side of the central line (10)

In this case the analyst can report the analytical results but a problem may be developing. Important trends should be discovered as early as possible in order to avoid serious problems in the future. Examples of important trends are when the majority of the control values lie far away from the central line though still within the warning limits. **In other words, each laboratory has to decide in the quality manual how to treat these trends.**

3. The method is **out of control** if:

-  • the control value is outside the action limits
-  • the control value is between the warning and the action limit and at least one of the two previous control values is also between warning and action limit – the rule two out of three – see for example March 22 in Figure 10.

In this case normally no analytical results can be reported. All results since last value in control was obtained must be reanalysed.

Out-of control situations

It is difficult to give general guidelines for how the laboratory should act when the analysis is out of control. The different analytical variables cannot be treated exactly in the same manner. The experience and common sense of the analyst is of vital importance when choosing remedial actions. However, if an out-of control situation occurs, it is most likely that there is an error also in the analyses of test samples.

If there is an out of control situation the normal action is to do some more (at least two) control analyses. If the new control values are located within the warning limits the routine samples can be reanalysed. If the control values are still outside the warning limits, the routine analyses shall be stopped, and remedial actions have to be taken to find and eliminate the cause(s) of error.

Controlling the reagents and the calibration of the method or exchange of vessels and apparatus are usual remedial actions in out-of control cases. The problem, and the solution of this, should be documented. Analyses which have been carried out since the last acceptable control value was obtained must, if possible, be repeated. If the repeated control values still are out of control the results of test samples shall not be reported. If the test samples cannot be re-analysed, for example due to instability, and the customer still urgently needs a result the laboratory can decide (after careful consideration) to report the value, provided that a clear note on the decreased reliability is given.

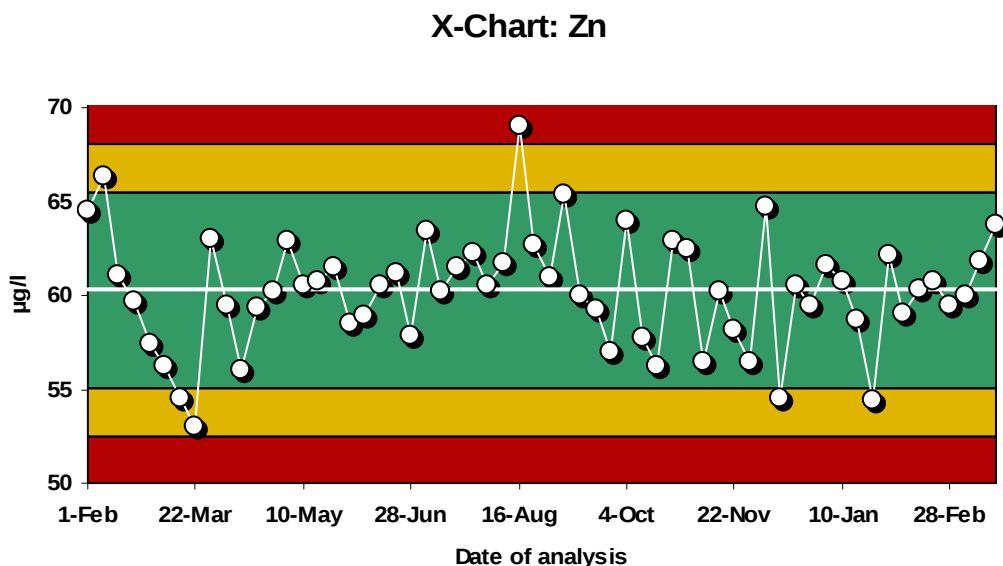


Figure 10. X control chart with two out of control situations.

10. Long-term evaluation of quality control data

This chapter is about using the quality control data from a period of time to answer two questions:

- *What is the quality (random and systematic effects) currently in the laboratory? Has the quality significantly changed?*
- *Are control limits and central line in the control chart still optimal for detecting situations out of control?*

Note: This is one of the most difficult tasks in QC and we can only give general guidance.

We will look at these two questions below.

Review of the current quality

This review is chiefly about statistical control limits and mean central line. The evaluation consists of a review of the last 60 data points on the control chart (10). Please note that some of these may also have been included in the previous evaluation, but there must be at least 20 **new** points. The review follows the following steps:

1. Count the number of cases where the results are outside the warning limits.. If this number is greater than 6 or less than 1 there is clear evidence (with 60 data points) that the spread of analysis has changed (10).
2. Calculate the mean of the last 60 results and compare with the previous mean value – the central line. If the difference is more than 0,35 s there is clear evidence (with 60 data points) that the mean value has changed.

How often should control limits be evaluated?

For successful use of control charts it is important that the control limits and the central line remain stable over a long period of time. The central line and control limits should not be changed frequently since this will make it difficult to detect gradual changes in analytical quality. The laboratory should have a policy for how often control limit are evaluated and how it is decided if a change is needed. We recommend that control limits and central line should be evaluated every year. For less frequent analyses, for example those performed once per month, we recommend evaluation after 20 control data have been collected.

You should not change control limits based on less than 20 new data since last evaluation because the uncertainty of the control limits will be too high, and you run the risk that control limits fluctuate in and out for no good reason.

What makes a change in control limits necessary?

Target control limits are only changed if customers' requirements change. This section is therefore only relevant for statistical control limits.

Control limits and central line should be evaluated every year or after collection of 20 data sets as indicated above. But the evaluation does not necessarily mean that the control limits should be changed. A change should only be considered if a significant change in spread or the bias has taken place.

If the review, points 1 and 2 above, has shown evidence of a change in spread or mean value we recommend making a statistical test to determine if the change is significant – see Chapter 14 Example 8. However even if the change is significant we do not recommend changing the central line unless there is a good explanation for the shift in data, e.g. a new control sample.

If an increase in spread is significant and if the change is acceptable compared to customers' requirements, calculate new warning and action limits as described in Chapter 7.

Special care must be taken when a control chart includes out-of control situations (see Chapter 9) in the 60 data points (or more) under consideration. This will happen now and then!. If an assignable cause for the out of control situation was identified at the time of the analysis, the control value should be excluded from the calculation of new control limits. However, there will inevitably be cases where out of control situations have existed but no assignable cause identified. These data could probably be the result of an undetected mistake for that particular batch of analyses and including them in calculations may lead to a falsely large standard deviation. On the other hand excluding such data, especially if there is more than one in the data set, may lead to a too optimistic standard deviation and falsely contract the control limits, leading to even more apparent out of control situations.

A pragmatic approach (10) is to exclude data that are more than 4 standard deviations away from the central line and retain the rest. If more than one out of control situation exists in the 60 points under consideration, it is more than you would expect and there is good reason to scrutinise the whole analytical procedure to search for the cause of the repeated out of control situations.

Review of spread and bias

The actual analytical quality produced in the laboratory is reviewed when reviewing control limits and central line.

If the review of the QC showed that there was no need to change the control limits and that the mean value was not changing, the analytical quality is unchanged and nothing further needs to be done, except to document the fact that a review has taken place.

If the review of control limits showed a need to change the limits, the analytical quality has changed. The new standard deviation for *within-laboratory reproducibility* and the mean is calculated, unless it has already been done to prepare new control limits for the X-chart. Laboratories using R-charts will also be able to calculate repeatability standard deviation. The new estimates must be compared to the requirements for quality using an F-test (standard deviations) or t-test (mean) and if acceptable, the laboratory's description of the quality updated. Equations are given in Chapter 12. The tests are performed as two-sided tests and it is customary to use 95% confidence levels. Example 8 in Chapter 14 illustrates the procedure.

11. Other uses of quality control data and control charts

The information obtained from the regular use of control charts can be used for other purposes than pure internal quality control. Depending on which type of control chart that is used, a few suggested uses are listed in this chapter.

Measurement uncertainty

Results from the control charts can, together with other data be used for calculating the measurement uncertainty. In most cases, the systematic effect and the random effect (the standard deviation) can be combined to calculate the measurement uncertainty. How this can be done is described in detail in Nordtest *Handbook for calculation of measurement uncertainty in environmental laboratories* (5) and also partly in Eurachem guide (6).

Measurement uncertainty is here estimated from control charts results combined with results from proficiency tests, data from method validations (or information given in standard methods). This approach provides a practical and general way of utilising already existing information. Provided the whole analytical chain is included in the control charts (i.e. also sample work-up such as filtration, concentration steps etc.) it may give a realistic estimate of the measurement uncertainty.

Method validation

Normally, a full method validation should be performed **before** a method is adopted in the laboratory. There might be situations, though, where a method is used after only partial validation, and where information from the control charts can be used to complement the available data. Such situations could occur if a method has been changed only slightly, or if a standard method is adopted directly from the literature.

- If a matrix CRM similar to routine samples is used in the control charts, the results will give direct information on the bias of the method, by comparing the resulting average result to the expected (certified) value. With an in-house or purchased standard, a rough estimate of the bias will be given, though with less certainty than when using a CRM.
- All types of control charts will provide information on the spread (random variation) from calculations of standard deviation or from estimates using the range.

Method comparison

Control charts can be used to compare different analytical methods using separate control charts for each method. This may for example give valuable method comparison information if the laboratory is in the process of changing from a manual to an automated method, or from a standard method to a non-standard method (e.g. a test-kit method). By running the two methods in parallel for some time, it is easily possible to compare important information such as:

- spread (from the standard deviation or from the range)
- bias (if a CRM is used)
- matrix effects (interferences), if spiking or a matrix CRM is used
- robustness, i.e. if one method is more sensitive to temperature shifts, handling etc.

Estimation of limit of detection (LOD)

The estimate of limit of detection used by many sectors is repeatability standard deviation multiplied by a factor. The factor is normally between 3 and 5. The repeatability standard deviation used in the calculation must be valid at low concentrations.

Data from an R-chart will give the repeatability standard deviation, and if the concentration is low, this standard deviation is useful for estimation of the limit of detection.

Data from an X-chart with a test sample at low concentration will also be useful for the estimation of the detection limit for the method in routine use.

Data from control sample type III (blank sample) may in some cases be used for the estimation, provided that the laboratory has evidence that the standard deviation for the blank is representative for the standard deviation for test samples with low concentration.

Person comparison or qualification

In the same way as for methods, it is possible to compare the performance of different persons in the laboratory. Whereas this might be very close to undesired policing, there is no doubt that control charts can be very useful tools when training and qualifying new staff in the laboratory. Part of the training activity will then be to plot results from control samples analysed by the person under training in control charts and to set target values for allowable systematic effect and spread, in comparison to what is reached by the already qualified staff. This way, the laboratory manager as well as the person trained will have a very objective tool for judging when the performance in the analytical work is sufficient to fulfil the requirements..

Evaluation of proficiency tests

If the laboratory regularly participates in proficiency tests of similar nature, plotting the PT results in control charts (similar to an X-chart) provides the quality manager with a good overview over the performance, including possible systematic effects or trends.

Here the z-score is plotted in an X-chart. Normally CL = 0, WL = 2 and AL = 3.

$$z = \frac{(x_{lab\ value} - x_{assigned\ value})}{s} \text{ or } zeta = \frac{(x_{lab\ value} - x_{assigned\ value})}{\sqrt{u_{lab}^2 + u_{assigned\ value}^2}}$$

Example: The total standard deviation in a proficiency test (all laboratories) was 0.08 mg/kg and your result was 0.12 mg/kg lower than the assigned value. Your z-score becomes -1.5. Here we recommend that all values outside warning limits should be investigated. The maximum allowed error from authorities (see also Chapter 3) can also be used to calculate the z-score.

Another possibility is the zeta score using your own claimed measurement uncertainty (u_{lab}) where u_{lab} is the combined standard uncertainty (6).

Environmental parameters and similar checks

When monitoring environmental parameters in the laboratory, such as the temperature in the laboratory or in the refrigerators, it is very useful and easy to use a simple type of target control chart for plotting the values. In such cases the ideal, expected, temperature will be used as the central line, and the allowable limits used as action limits. The control charts give a very simple graphical presentation of any trends or unexpected variation that might influence the analyses and therefore might be worth considering.

Similarly, it is useful to plot the results of the frequent verification of the analytical balance or other regular checks, partly to detect any trends in the material, but also to see easily if the results are outside or inside the permissible limits.

12. Terminology and Equations

Here we try to describe the statistical equations and terms we use in this handbook in a clear way. Exact definitions for terms used are found in VIM Ref (13). Direct quote from this reference are given below in italics. All terms defined here are given in bold text

Terminology

Accuracy of measurement

*The closeness or the agreement between the result of a measurement and a true value of the measurand (13). The accuracy is affected by both **systematic** and random effects.*

Analyte

The substance or parameter subject to measurement.

Analytical run - batch of analyses

Analyses of a number of routine samples and **control samples**. Normally one **control value** for each batch is entered into each **control chart**.

Bias – systematic error

The difference between the accepted reference value and the **mean value** of a great number of test results (*Figure 6*).

Confidence interval

The range about the **mean value** within which a stated percentage of values would be expected to lie. For example, for a normal distribution, approximately 95 % of values are between $\pm 2 s$ (*Figure 7*).

Control chart

The principal tool in internal quality control. A chart where the **control values** are entered and compared with **control limits**.

Control limits

Limits in a **control chart**. There are two control limits: action limits (AL) and warning limits (WL).

Control sample

Sample material whose test results are used to construct **control charts**, e.g., standard solutions, test samples, blank samples.

Control value

Test result from the internal quality control entered in the **control chart**. It can, e.g. be a single value, a mean value or a range. These values are reported different from test results - values from analyses of routine sample: Control values are reported with one extra significant figure and also negative values are reported, e.g. a control value – 0,07 mg/l in a X-chart could for a routine sample be reported $< 0,1$ mg/l.

Degrees of freedom, df

The number of independent comparisons that may be made between individual results in a set. In general terms the number of degrees of freedom, e.g. for an estimated standard deviation, provides an indication of the reliability of the estimate. As the number of degrees of freedom increases, the random error of the estimate itself, s , decreases. The degrees of freedom are used when comparing statistical quantities, see F- and t-test below.

Detection limit

The lowest concentration of an **analyte** that can, with a given probability, be detected with a specified method.

Limit of Quantification

When an analytical result is below this limit it is reported as less than (<). Another term used is Reporting limit.

Measurand

Quantity intended to be measured, e.g. the amount of acid-soluble cadmium (the **analyte**) in a fresh-water sample.

Measurement procedure

The detailed description of an analytical method used in a laboratory.

Measurement uncertainty

Parameter, associated with the result of a measurement that characterizes the dispersion of the values that could reasonably be attributed to the **measurand** (13). Measurement uncertainty can be interpreted as a quantitative estimate of **accuracy** (**trueness** + precision) – see *Figure 3*.

Outlier rejection

In the statistical calculation we recommend to reject outliers that are more than 4 s different from the mean (10). This is a practical approach. Another alternative is to use Grubbs test – see statistical textbooks.

Repeatability

The degree of agreement between independent test results of repeated determinations of a sample with the same method and under identical conditions, *e.g. same instrument, operator and within a short interval of time*. The whole procedure should be repeated from taking a new test portion of a sample to the final reading or calculation of result.

Reproducibility

The degree of agreement between individual results determined on a sample with the same method, but varying conditions, e.g. time, analyst, laboratory.

Within-laboratory reproducibility (Intermediate precision)

The degree of agreement between individual results determined in a laboratory on a sample with the same measurement procedure over a long time period i.e. at least a year. The time period could be shorter if enough data is collected but in many cases a year is suitable to encompass all variations in reagents, personnel, instrument service etc.

Test result (response value)

The value obtained by applying the measurement procedure. The **control value** entered in the **control chart** is either the test result of a **control sample** (reported with one more significant figure and not less than) or a value calculated from the test results e.g. the range. Dependent on the type of **control sample**, maybe only a part of the measurement procedure can be applied to the control sample.

Spread

The variation between independent test results obtained under stipulated conditions. The opposite is closeness of agreement between test results - also called precision

Systematic effect (bias)

The difference between the accepted reference value and the **mean value** of a great number of analytical results.

Trueness

Closeness of agreement between the **mean value** obtained from a large series of **test results** and an accepted reference value. Trueness is normally expressed in terms of **bias (systematic effect)**.

Equations

Mean value ($\bar{x}$)

The sum of every individual result (x_i), divided by the number (n) of results:

$$\bar{x} = \frac{\sum x_i}{n} \quad 1)$$

Standard deviation (s).

A measure for the **spread** of individual results (x_i) around the **mean value** ($\bar{x}$):

$$s = \sqrt{\frac{\sum (x_i - \bar{x})^2}{(n-1)}} \quad 2)$$

Degrees of freedom, $df = n - 1$

Coefficient of variation (CV). The standard deviation expressed in relative percent of the **mean value**:

$$CV (\%) = \frac{100 \cdot s}{\bar{x}} \quad 3)$$

Standard deviation from range ($n=2$). Calculated for the application of R-charts (Range is here the difference between the two values): For values of n from 3 to 5 see Chapter 13 *Table 4*.

$$s = \frac{Range}{1,128} \quad (n = 2) \quad 4)$$

F-test

(see Chapter 13, *Table 3*). Used to evaluate whether the **standard deviations** (s_1 and s_2) from two series of determinations are significantly different:

$$F = s_1^2 / s_2^2, \quad s_1 > s_2 \quad 5)$$

When the calculated F-value is greater than the critical F-value found in *Table 3*, the two standard deviations are significantly different.

t-test

(see Chapter 13, *Table 2*). Used to evaluate whether there is a significant difference between the **mean value** ($\bar{x}$) for a series of determinations and the accepted reference value (T):

$$t = \frac{|\bar{x} - T|}{s} \cdot \sqrt{n} \quad 6)$$

alternatively, between the mean values ($\bar{x}_1$ and $\bar{x}_2$) of two different series of analyses:

$$t = \frac{|\bar{x}_1 - \bar{x}_2|}{s_c} \cdot \sqrt{\frac{n_1 \cdot n_2}{(n_1 + n_2)}} \quad 7)$$

where s_c is the combined **standard deviation**, see formula 9).

When the calculated t-value is greater than the critical t-value found in *Table 2*, the difference between the two values is statistically significant.

Combined mean ($\bar{x}_C$) for several series of analyses

Calculated from the mean values for k series of analyses with total of $n_1+n_2+\dots=n_{tot}$ observations:

$$\bar{x}_C = \frac{n_1 \cdot \bar{x}_1 + n_2 \cdot \bar{x}_2 + \dots + n_k \cdot \bar{x}_k}{n_{tot}} \quad 8)$$

Combined (pooled) standard deviation (s_C) for several series of analyses. Calculated from the standard deviations for k series of analyses with total of $n_1+n_2+\dots=n_{tot}$ observations:

$$s_C = \sqrt{\frac{(n_1 - 1) \cdot s_1^2 + (n_2 - 1) \cdot s_2^2 + \dots + (n_k - 1) \cdot s_k^2}{n_{tot} - k}} \quad 9)$$

Degrees of freedom, $df = n_{tot} - k$.

If n is about the same for the different series

$$s_C = \sqrt{\frac{s_1^2 + s_2^2 + \dots + s_k^2}{k}} \quad 10)$$

Detection limit (LOD). Is normally set to between 3 s and 5 s. The **standard deviation, s**, is the repeatability standard deviation valid at low concentration.

13. Tables

First table in this section in Table 2. Table 1 you can find on page 5.

Table 2. Critical *t*-values (2-sided test).

Degrees of freedom	Confidence level (%)				Degrees of freedom	Confidence level (%)			
	90	95	99	99.9		90	95	99	99.9
1	6,31	12,7	63,7	637	21	1,72	2,08	2,83	3,82
2	2,92	4,30	9,92	31,6	22	1,72	2,07	2,82	3,79
3	2,35	3,18	5,84	12,9	23	1,71	2,07	2,81	3,77
4	2,13	2,78	4,60	8,61	24	1,71	2,06	2,80	3,75
5	2,01	2,57	4,03	6,86	25	1,71	2,06	2,79	3,73
6	1,94	2,45	3,71	5,96	26	1,71	2,06	2,78	3,71
7	1,89	2,36	3,50	5,41	27	1,70	2,05	2,77	3,69
8	1,86	2,31	3,36	5,04	28	1,70	2,05	2,76	3,67
9	1,83	2,26	3,25	4,78	29	1,70	2,05	2,76	3,66
10	1,81	2,23	3,17	4,59	30	1,70	2,04	2,75	3,65
11	1,80	2,20	3,11	4,44	35	1,69	2,03	2,72	3,59
12	1,78	2,18	3,05	4,32	40	1,68	2,02	2,70	3,55
13	1,77	2,16	3,01	4,22	45	1,68	2,01	2,69	3,52
14	1,76	2,14	2,98	4,14	50	1,68	2,01	2,68	3,50
15	1,75	2,13	2,95	4,07	55	1,67	2,00	2,67	3,48
16	1,75	2,12	2,92	4,02	60	1,67	2,00	2,66	3,46
17	1,74	2,11	2,90	3,97	80	1,67	1,99	2,64	3,42
18	1,73	2,10	2,88	3,92	100	1,66	1,98	2,63	3,39
19	1,73	2,09	2,86	3,88	120	1,66	1,98	2,62	3,37
20	1,72	2,09	2,85	3,85	∞	1,64	1,96	2,58	3,29

Table 3. Critical F-values at the 95% confidence level (2-sided test) for df from 4 to 120.

Values of $F_{1-\alpha}(df_1, df_2)$, $\alpha = 0,025$														
df ₁	4	5	6	7	8	10	12	15	20	24	30	40	60	120
df ₂														
4	9,60	9,36	9,20	9,07	8,98	8,84	8,75	8,66	8,56	8,51	8,46	8,41	8,36	8,31
5	7,39	7,15	6,98	6,85	6,76	6,62	6,52	6,43	6,33	6,28	6,23	6,18	6,12	6,07
6	6,23	5,99	5,82	5,70	5,60	5,46	5,37	5,27	5,17	5,12	5,07	5,01	4,96	4,90
7	5,52	5,29	5,12	4,99	4,90	4,76	4,67	4,57	4,47	4,42	4,36	4,31	4,25	4,20
8	5,05	4,82	4,65	4,53	4,43	4,30	4,20	4,10	4,00	3,95	3,89	3,84	3,78	3,73
10	4,47	4,24	4,07	3,95	3,85	3,72	3,62	3,52	3,42	3,37	3,31	3,26	3,20	3,14
12	4,12	3,89	3,73	3,61	3,51	3,37	3,28	3,18	3,07	3,02	2,96	2,91	2,85	2,79
15	3,80	3,58	3,41	3,29	3,20	3,06	2,96	2,86	2,76	2,70	2,64	2,59	2,52	2,45
20	3,51	3,29	3,13	3,01	2,91	2,77	2,68	2,57	2,46	2,41	2,35	2,29	2,22	2,14
24	3,38	3,15	2,99	2,87	2,78	2,64	2,54	2,44	2,33	2,27	2,21	2,15	2,08	2,01
30	3,25	3,03	2,87	2,75	2,65	2,51	2,41	2,31	2,20	2,14	2,07	2,01	1,94	1,87
40	3,13	2,90	2,74	2,62	2,53	2,39	2,29	2,18	2,07	2,01	1,94	1,88	1,80	1,72
60	3,01	2,79	2,63	2,51	2,41	2,27	2,17	2,06	1,94	1,88	1,82	1,74	1,67	1,58
120	2,89	2,67	2,52	2,39	2,30	2,16	2,05	1,94	1,82	1,76	1,69	1,61	1,53	1,43

df1 = degrees of freedom in numerator (s_1^2), df2 = degrees of freedom in denominator (s_2^2)

Table 4. Factors for estimation of standard deviation from mean range, and calculation of central line, warning and action limits for construction of R-charts (9).

Number of replicates	Standard deviation s	Central line CL	Warning limit WL	Action limit AL	¹ Mean Range $= \frac{\sum (Max - Min)}{n_{samples}}$
	Mean range/ ¹ d_2	$d_2 \cdot s$	$D_{WL}^2 \cdot s$	$D_2 \cdot s$	² Calculated from $D_{WL} = d_2 + \frac{2}{3}(D_2 - d_2)$ Formula originally developed for this handbook
2	Mean range/1,128	1,128•s	2,833•s	3,686•s	
3	Mean range/1,693	1,693•s	3,470•s	4,358•s	
4	Mean range/2,059	2,059•s	3,818•s	4,698•s	
5	Mean range/2,326	2,326•s	4,054•s	4,918•s	

Comments

Confidence levels for the control limits in X and R-charts

The action limit ($\pm 3 s$) for X-chart is for a normal distribution with a confidence level of 99,73 %. Using uncertainty propagation the action limit for R-chart based on duplicates at the same confidence level would be $4,25 (\pm 3 \cdot \sqrt{2} = 4,25 \cdot s)$. However in the ISO standard 8258 for control charts (9) the factor given is 3,686. Using the factor of 3,686 a confidence level for a normal distribution will be 99,1 % (using the statistical table over the standard normal cumulative distribution function for $z \pm 3,686/\sqrt{2}$). This is what is normally used and works well.

The warning limits for R-charts calculated with our proposed equation here is with the same confidence level (about 95,5 %) as for X-charts.

Different factors for calculating control limits

If the mean range is used directly for calculation of the warning and action limits instead of the standard deviation, the factors are e.g. in case of two replicates: 2,512 and 3,268 (2,833/1,128) and 3,686/1,128).

14. Examples

In this Chapter we will give examples of different control charts from different sectors. All examples are data taking from the authors' laboratories. The yearly reviewing of the control limits are described in detail in example 8.

Example 1

Determination of Ni in low-alloy steel with X-Ray Fluorescence (XRF)


Sample type	Control chart	Control limits	Central line
Steel sample – routine sample	X-chart	Target	Mean value

High concentration of nickel. The mean value for our control values over one year is 4,58 % (abs)⁶ with a standard deviation of 0,026 % (abs). The control sample is covering the whole measurement procedure (polishing and measurement).

The requirement on expanded measurement uncertainty⁷ (U) is 4 % (rel). This will be 2 % (rel) as standard uncertainty u_c . The requirement of s_{Rw} can normally be set to half or 50 % of the standard uncertainty⁸ so we obtain an estimate of the requirement from

$$s_{Rw} = \frac{u_c}{2} = \frac{U}{4} = \frac{4\%(rel)}{4} = 1\%(rel) \text{ or } 0,0458 \% (abs)$$

From the requirement on s_{Rw} we calculate the target control limits.

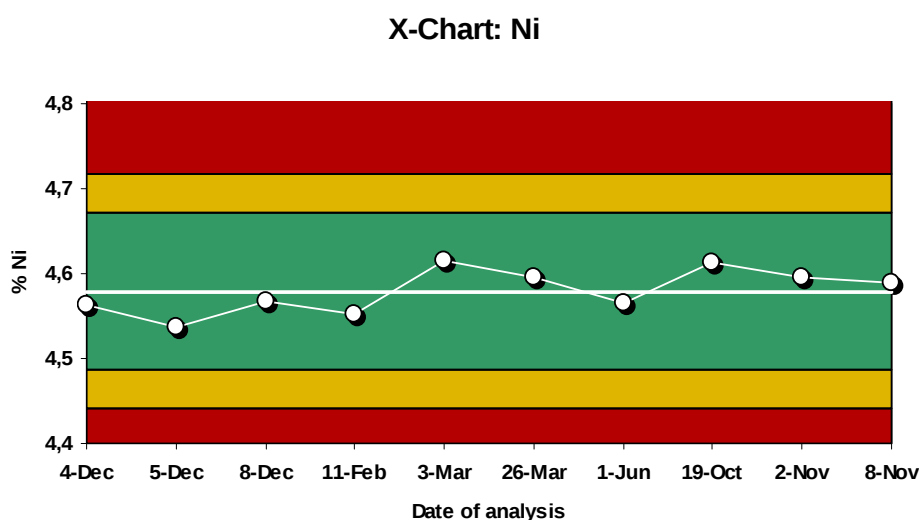

$$\bar{x} = 4,58 \% (abs)$$

$$s_{target} = 0,0458 \% (abs)$$

$$CL: 4,58 \% (abs)$$

$$WL: 4,58 \pm 2 \cdot 0,0458 = 4,67 \text{ and } 4,49 \% (abs)$$

$$AL: 4,58 \pm 3 \cdot 0,0458 = 4,72 \text{ and } 4,44 \% (abs)$$

⁶ The X-chart concentration unit is in weight % of nickel (% abs) and the demand is given in relative percent of the nickel value (% rel).

⁷ Further information on expanded and standard uncertainty is available in the Eurachem/CITAC guide (6).

⁸ Due to the way standard deviations are added this will result in a 25 % **contribution** to the standard uncertainty.


Example 2

Determination of Co in low-alloy steel with XRF

Sample type	Control chart	Control limits	Central line
Steel sample – routine sample	X-chart	Target	Mean value

Low concentration of cobalt. The mean value for our control values over one year is 0,0768 % (abs)⁹ with a standard deviation of 0,00063 % (abs). The control sample is covering the whole measurement procedure (polishing and measurement).

The requirement for limit of quantification LOQ is 0,01 % (abs) and this is normally set to 6 to 10 times the standard deviation of a blank or a sample at low concentration. This will require 0,001 % (abs) as a standard deviation and this value can be used to set the control limits. From the limit of quantification (LOQ) we therefore calculate the control limits to be:

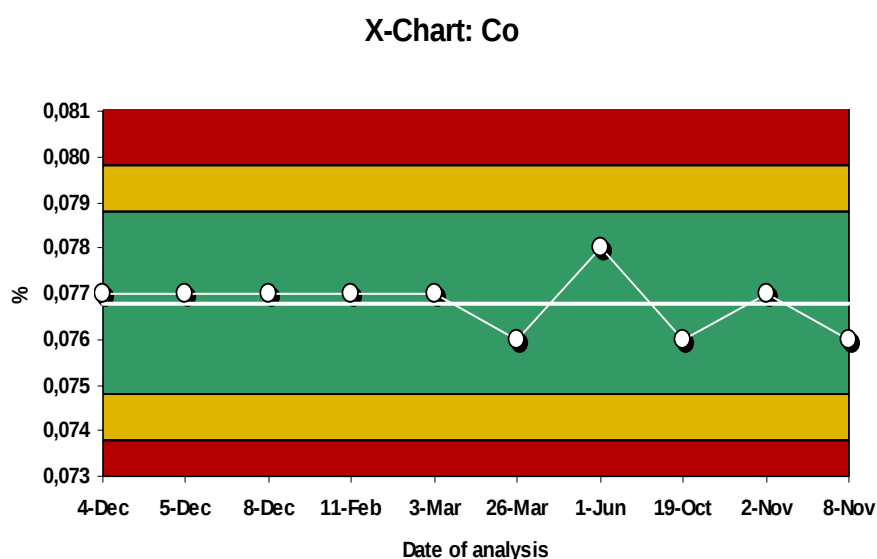

$$\bar{x} = 0,0768 \% \text{ (abs)}$$

$$s_{\text{target}} = 0,001 \% \text{ (abs)}$$

$$\text{CL: } 0,0768 \% \text{ (abs)}$$

$$\text{WL: } 0,0768 \pm 2 \cdot 0,001 = 0,0788 \text{ and } 0,0748 \% \text{ (abs)}$$

$$\text{AL: } 0,0768 \pm 3 \cdot 0,001 = 0,0798 \text{ and } 0,0738 \% \text{ (abs)}$$

Comment

The concentration of the control sample is 8 times the LOQ. In this case this reflects the concentration of interest and is therefore suitable.

⁹ See footnote 6 on page 35.

Example 3

Determination of N-NH₄ in water with indophenol blue method



Sample type	Control chart	Control limits	Central line
Standard solution	X-chart	Statistical	Mean value
Standard solution	R –chart	Statistical	Mean range value

Low concentration (20 µg/l) in a synthetic solution. (NH₄)₂SO₄ was used for preparation of the stock solution of 100 mg/l, and from this the control sample was prepared. The stock solution was different from the solution used for preparation of the calibration standards (which is prepared from NH₄Cl). The control sample was used for analyses of waters in the concentration range between 2 µg/l and 100 µg/l.

The control was performed as duplicates.

The X-chart and R-chart were established as follows:

- The mean value of the duplicates was used for plotting of X-chart and the mean value of all results was used as the central line (CL). The standard deviation was used for calculating the control limits.
- The range value of the duplicates was used for plotting of the R-chart. The mean range was used as the central line (CL). The standard deviation (estimated from the range) was used for calculating the control limits.

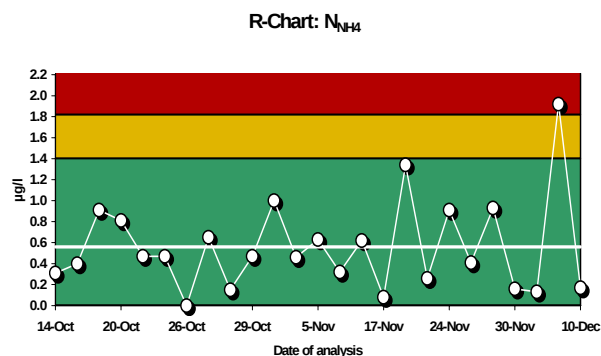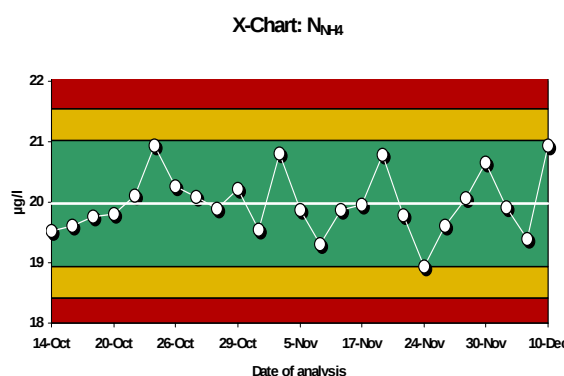

$\bar{x} = 19,99 \text{ µg/l}$ and $s = 0,521 \text{ µg/l}$ CL: 19,99 µg/l WL: $19,99 \pm 2 \cdot 0,521 = 19,99 \pm 1,04 \text{ µg/l}$ (18,95 & 21,03 µg/l) AL: $19,99 \pm 3 \cdot 0,521 = 19,99 \pm 1,56 \text{ µg/l}$ (18,43 & 21,55 µg/l)	Mean range = 0,559µg/l and $s = 0,559/1,128 = 0,496 \text{ µg/l}$ CL: 0,559 µg/l WL: $2,83 \cdot 0,496 = 1,40 \text{ µg/l}$ AL: $3,67 \cdot 0,496 = 1,82 \text{ µg/l}$
---	---

Comment

On the X-chart the mean value was same as the calculated concentration 20 µg/l – no systematic effects were obtained in analyses. There were no results that exceeded the control limits (Chapter 9). On the R-chart there was one control value that exceeded the action limit. The control sample as well as the test samples were reanalysed on 10 Dec with positive outcome. This control value outside the action limit should therefore be rejected when reviewing the R-chart (Chapter 9 and 10).

Example 4


Determination of Pb in water with ICP-MS

Sample type	Control chart	Control limits	Central line
In-house lake water	X-chart	Statistical	Mean value

Low concentration of Pb (0,29 µg/l) in an in-house material. The control sample was prepared from lake water for analysis of low concentrations of Pb (< 1 µg/l) in waters. The sample was preserved with HNO₃. The control was performed once in each analytical run.

The X-chart was established as follows:

- The individual results were used for plotting of X-chart
- The mean value of all results was used as the central line (CL)
- The standard deviation was used for calculating the control limits

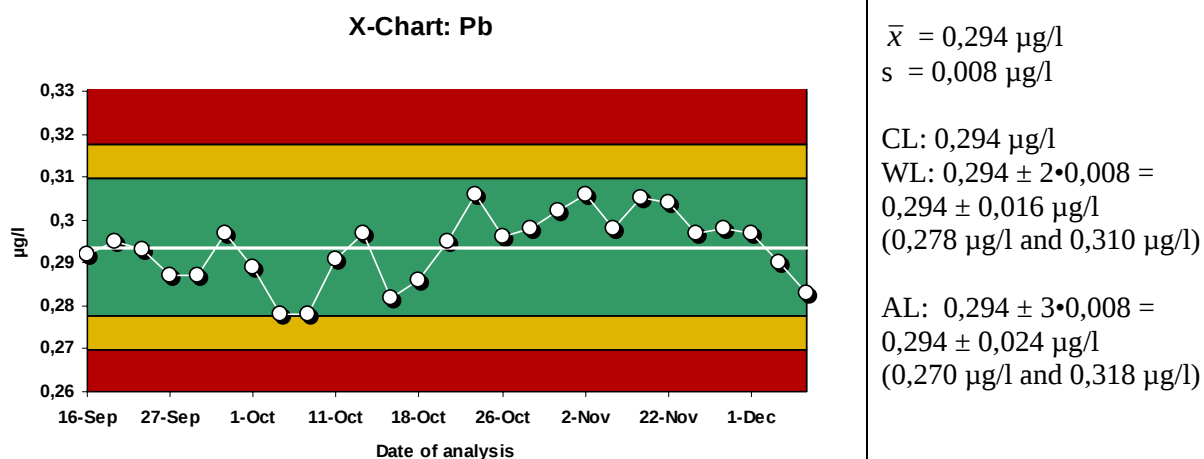

Comment

On the X-chart the control values were within the limits. No systematic effects were detected in the results.

There are 12 consecutive results above the central line. This is out of statistical control but as described in Chapter 9 regarded as acceptable.

Example 5


Determination of As in biological material with ICP-MS

Sample type	Control chart	Control limits	Central line
CRM	X-chart	Target	Certified value

High concentration of As ($18 \mu\text{g/g}$) in the CRM (Dogfish muscle NRC/DORM-2). The control sample was used for the determination of As in biological material. The sample was analysed once in each run.

The X-chart was established as follows:

- The individual results were used for plotting of X-chart
- The certified value was used as the central line (CL)
- The target standard deviation of 5 % was used to calculate the control limits

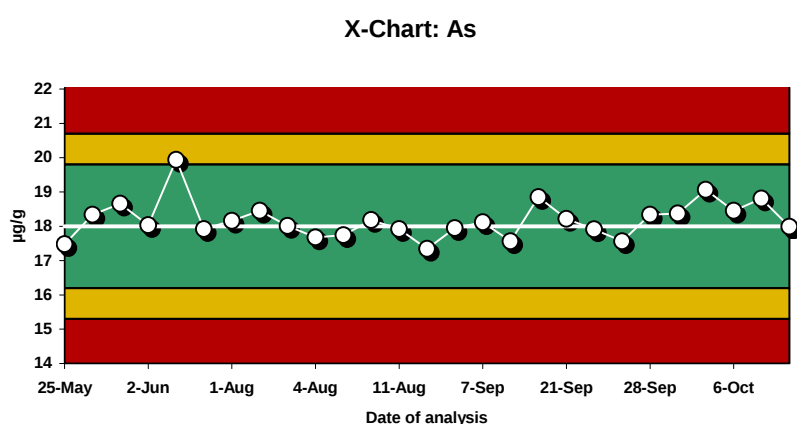

Certified value = $18,0 \mu\text{g/g}$
 $S_{\text{target}} = 0,05 \cdot 18,0 = 0,9 \mu\text{g/g}$

CL: $18,0 \mu\text{g/g}$

WL: $18,0 \pm 2 \cdot 0,9 =$
 $= 18,0 \pm 1,8 \mu\text{g/g}$
 ($16,2 \mu\text{g/g}$ and $19,9 \mu\text{g/g}$)

AL: $18,0 \pm 3 \cdot 0,9 =$
 $= 18,0 \pm 2,7 \mu\text{g/g}$
 ($15,3 \mu\text{g/g}$ and $20,7 \mu\text{g/g}$)

Comment

On the X-chart there was one control value exceeded the warning limit. However, the previous value and the next one were both within the warning limits – the method was in control (Chapter 9).

Example 6


Determination of total P in water using spectrophotometric method

Sample type	Control chart	Control limits	Central line
Routine samples	r%-chart	Statistical	Mean relative range

Routine samples (10 - 50 µg/l) According to method validation the detection limit (3 s) was 2 µg/l. In each run one test sample was analysed as duplicates. The results were applied for r%-charting.

The r%-chart was established as follows:

- The difference of duplicates as percent of the mean value was used for plotting
- The mean of the r%-values was used as the central line (CL).
- The standard deviation of the r%-values was used for calculating the control limits

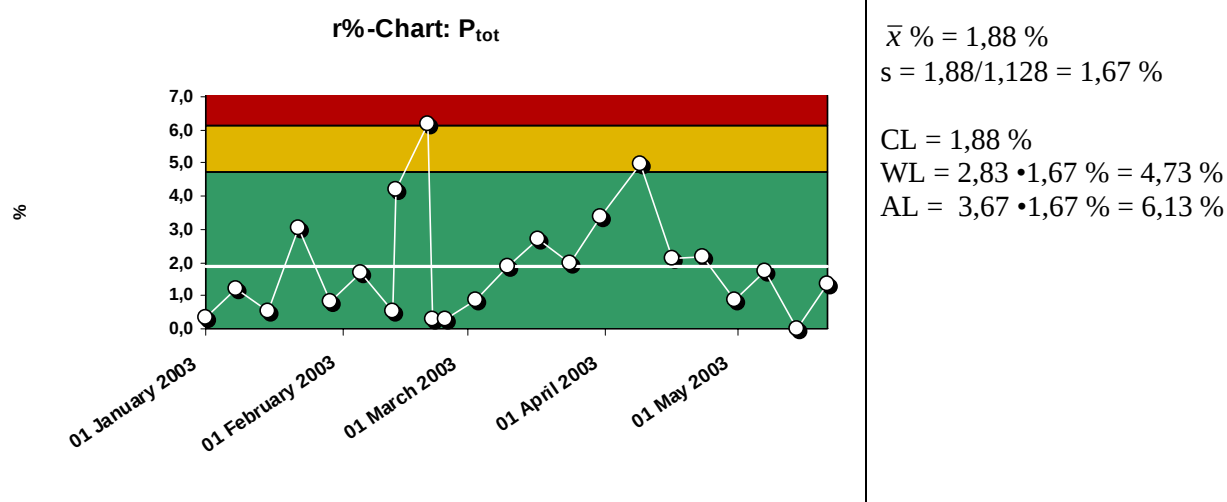

Comment

In the r%-chart two control values (series 9 and 17) exceeded the control limit. In the series 17 the warning limit was exceeded and in the series 9 the action limit was exceeded. In the series 9 the repeatability was out of control (Chapter 9) and after taking care of the problem this sample and the test samples were reanalysed (series 10).

Example 7


Determination of b-HCH (b- hexachlorocyclohexane) in biological material with Gas Chromatography

Sample type	Control chart	Control limits	Central line
CRM	X-chart	Target	Reference value

Cod liver oil BCR/598 with b-HCH (16 µg/kg). The control sample was used for analysis of b-HCH in biological material. The sample was analysed once in each run.

The X-chart was established as follows:

- The individual results were used for plotting of X-chart.
- The certified value was used as the central line (CL).
- The target standard deviation of 15 % was used to calculate the control limits

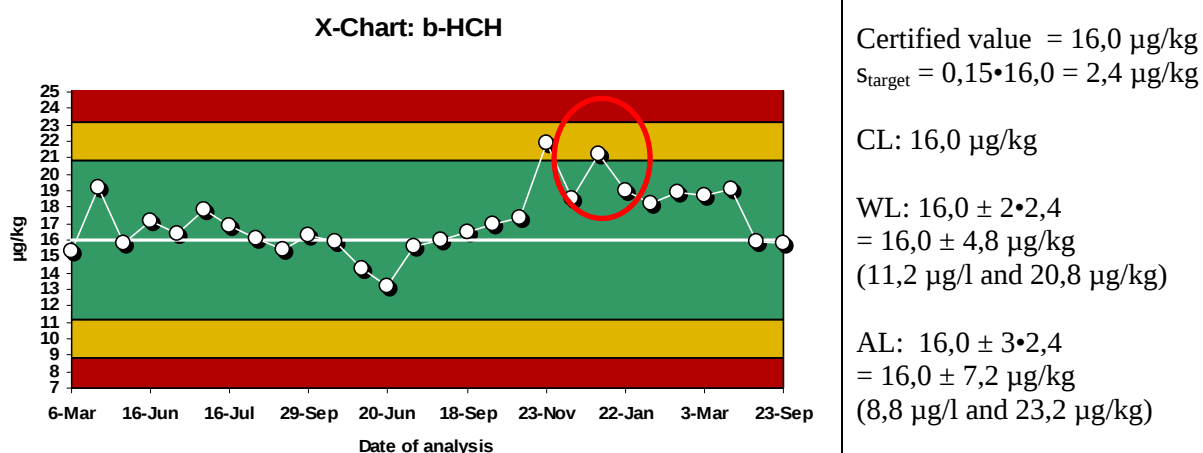

Comment

A trend was detectable in the results: From September 11 results were above the CL and once two control values out of three were above the warning limit. This time (about 1st of January) the analyses were out of control,

Example 8

Determination of Cu in water with ICP-OES

Sample type	Control chart	Control limits	Central line
In-house synthetic standard	X- and R-charts	Statistical	Mean value

In-house synthetic standard ($1,00 \pm 0,02$ mg/l). The control sample was prepared from a commercial standard. The sample was preserved with HNO₃. Control was performed twice in each analytical run.

X- and R-charts were established in 2003. Preliminary control limits and central line were estimated from the first 60 analytical runs.

X-chart:


- The average of the results for the control sample in each run was plotted.
- The mean value was used as the central line (CL).
- The standard deviation was used for calculating the control limits.

R-chart:

- The range for duplicates (highest value minus lowest value) was used for plotting.
- The mean range for the same 60 analytical runs that were used to establish the X-chart was used as the central line.
- The repeatability standard deviation (s_r) calculated from the mean range was used to establish control limits by multiplication with factors D_{WL} and D_2 (Chapter 13, Table 4).

The control charts were established and analyses were continued.

:

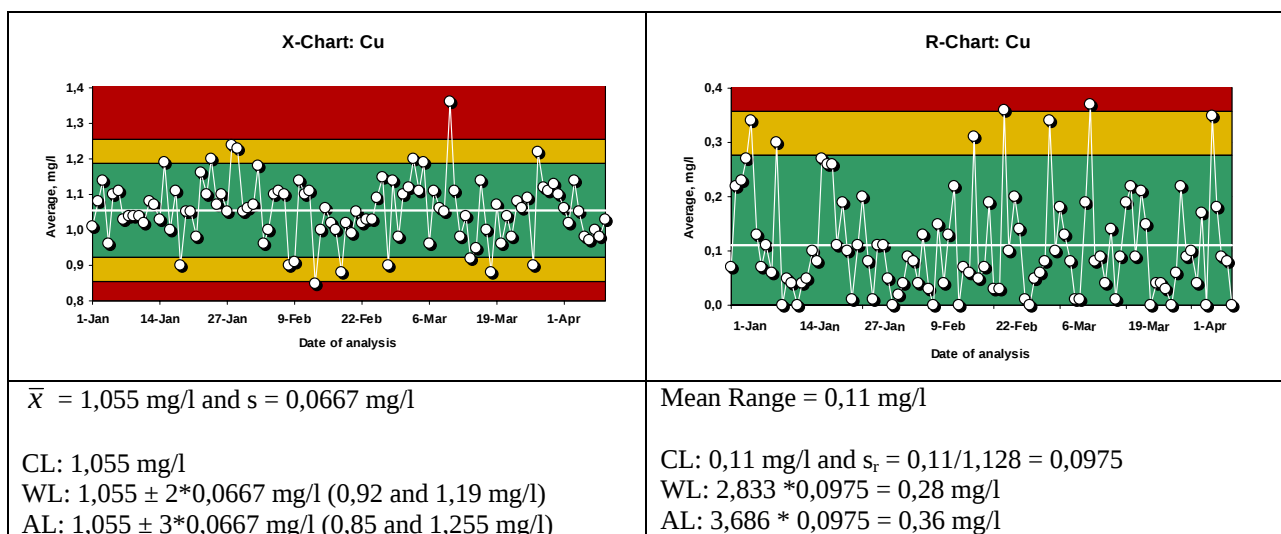

Review of the data

It is now time for the review of the control charts. As described in Chapter 9 we look at the last 60 data. These are the data plotted since 9 February 2004.

We count the number of times that the control values were outside the warning limits **since** 9 February (the vertical line in the X-chart). On the X-chart we find three cases where the upper warning limit is **clearly** exceeded, one of these even outside the action limit, and seven cases clearly below the lower warning limit. This makes a total of 10 times where the warning limits have been exceeded. There is thus reason to change the preliminary control limits. On the R-

chart we find five cases outside the warning limit. This is less than the required number of more than six times but we will review the limits in both control charts anyway.

The control value on the X-chart on 11 March was outside the upper action limit. On this date the results of routine analyses were rejected and the routine samples were afterwards re-analysed. This control value is regarded as an outlier because it differs from the central line by more than 4 standard deviations; see discussion on outliers in Chapter 10. We have therefore excluded this point from all statistical analysis of the data.

We calculate a new average and standard deviation from the last 59 points on the X-chart (only 59 since the outlier has been excluded) and a new average range for the last 60 points on the R-chart.

New $\bar{X}$ = 1,041 mg/l and new s = 0,0834 mg/l	New R = 0,108 mg/l
--	----------------------

X-chart

We compare the new standard deviation to the original standard deviation using an F-test:

$$s_{\text{new}}^2 / s_{\text{original}}^2 = 0,0834^2 / 0,0667^2 = 1,563$$

The s values have 59 and 58 degrees of freedom since they are based on 60 and 59 data points.

In Chapter 13, *Table 3* we can not find 58 or 59 degrees of freedom, but we can find 60. Since the difference between the values in the table for 40 and 60 degrees of freedom is small we do not bother to interpolate. Using 60 degrees of freedom for df_1 (new s) and df_2 (original s) we find that the critical value for F is 1,67. This is larger than our calculated value for F (1,563) and therefore the new s is not significantly higher than the original value for s . However, this F value is close to the critical value as would be expected from the number of times that the warning limits are exceeded (10 times with 60 data points). Since there was not a significant change we recommend recalculating the control limits based on all the data. It is always good to have well determined control limits based on as long a period as possible, preferably over a year.

We will now investigate if the central line has changed significantly. This we do using a t-test. The equation in Chapter 12 is:

$$t = \frac{|\bar{X}_1 - \bar{X}_2|}{s_C} \cdot \sqrt{\frac{n_1 \cdot n_2}{n_1 + n_2}}$$

This equation uses s_C , which is the combined standard deviation for the two sets of data giving the original and the new mean value. The equation for calculation of s_C is also given in Chapter 12:

$$s_C = \sqrt{\frac{(n_1 - 1) \cdot s_1^2 + (n_2 - 1) \cdot s_2^2 + \dots + (n_k - 1) \cdot s_k^2}{n_{\text{tot}} - k}} =$$

$$\frac{(60 - 1) \cdot 0,0667^2 + (59 - 1) \cdot 0,0834^2}{(60 + 59 - 2)} = 0,07545 \text{ mg/l}$$

Since s_C is now based on both sets of data it has $59 + 58 = 117$ degrees of freedom.

$$t = \frac{|1,055 - 1,041|}{0,07545} \cdot \sqrt{\frac{60 \cdot 59}{60 + 59}} = 1,012$$

In Chapter 13, *Table 2* we find the critical value for the t-test at 95% confidence level. The critical value is the same for 100 and 120 degrees of freedom and therefore also for 117 degrees of freedom: 1,98. The calculated t-value in our test is small compared to the critical value and

therefore we see no significant difference between the central line (original mean value) and the mean for the last 60 data points.

Previous preliminary X-chart	New X-Chart based on longer time period
$\bar{x} = 1,055 \text{ mg/l}$ and $s = 0,0667 \text{ mg/l}$	$\bar{x} = 1,048 \text{ mg/l}$ and $s = 0,0822 \text{ mg/l}$
CL: 1,055 mg/l	CL: 1,048 mg/l
WL: $1,055 \pm 2 \cdot 0,0667 \text{ mg/l}$ (0,92 and 1,19 mg/l)	WL: $1,052 \pm 2 \cdot 0,0822 \text{ mg/l}$ (0,888 and 1,217 mg/l)
AL: $1,055 \pm 3 \cdot 0,0667 \text{ mg/l}$ (0,85 and 1,255 mg/l)	AL: $1,052 \pm 3 \cdot 0,0822 \text{ mg/l}$ (0,806 and 1,300 mg/l)

R-chart

In the R-chart we have the central line equal to the mean range from the original data. The mean range is proportional to the repeatability standard deviation (see Equation 4 in Chapter 12). We can therefore compare repeatability standard deviations by comparing mean ranges. Again we use the F-test:

$$F = r_{\text{original}}^2 / r_{\text{new}}^2 = 0,11^2 / 0,108^2 = 1,037$$

The critical value for F from *Table 3* in Chapter 13 is 1,67 (see further under x-chart). This is larger than our calculated value for F and therefore the repeatability standard deviation – and the range – has not changed significantly and we recommend recalculating the control limits based on all the data. The new calculation gave the same mean range so no changes to the R-chart.

Conclusion

These results show that the spread and bias of the analyses have not changed *significantly*. We have taken advantage of the larger data set to calculate new and more reliable control limits based on all available data.

However there is a 5% bias in comparison with the expected value of the control sample, a standard solution at a high level ($1,00 \pm 0,02 \text{ mg/l}$) and we would recommend investigating this and changing the procedure to reduce this bias.

Example 9

Determination of Zn in hydrogen peroxide with ICP-OES - blank samples


Sample type	Control chart	Control limits	Central line
A blank sample	X- chart	Statistical	Mean value

Blank sample of ultrapure water. The blank determination was carried out for check of contamination. In the procedure 50 ml H₂O is evaporated to near dryness, 0,5 ml acid added and diluted to 5 ml.

X-chart

- The mean value of the results was used as the central line (CL). The standard deviation was used for calculating the control limits.

X-Chart: Zn in blank samples

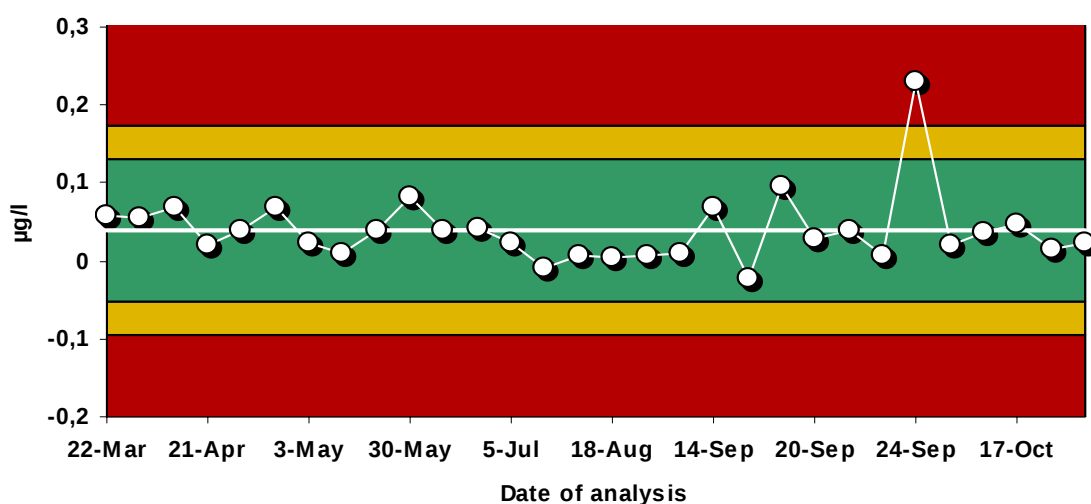

$$\bar{x} = 0,039 \text{ mg/l} \quad s = 0,045 \text{ mg/l}$$

$$\text{CL: } 0,039 \text{ mg/l}$$

$$\text{WL: } 0,039 + 2 \cdot 0,045: 0,129 \text{ mg/l} \quad \text{and} \quad -0,051 \text{ mg/l}$$

$$\text{AL: } 0,039 + 3 \cdot 0,045 = 0,174 \text{ mg/l} \quad \text{and} \quad -0,096 \text{ mg/l}$$

Comment

There was one result (24-Sep) that exceeded the action limit.

15. References

1. V. B. Jensen, K. Haapala, H. Hovind & Ö. Lindgren. *Handbook of internal quality control in water laboratories*. Copenhagen: Water Quality Institute, 1984 (in Danish).
2. H. Hovind: *Internal Quality Control. Handbook for Water Analysis Laboratories*. Oslo: Norwegian Institute for Water Research, 1986 (in Norwegian).
3. ISO / IEC 17025:2005 – *General requirements for the competence of testing and calibration laboratories*, Geneva: International Organization for Standardization; 2005.
4. E. Hund, D. Luc Massart, J. Smeyers-Verbeke. *Operational definition of uncertainty*, TRAC 2001; 20(8):394-406.
5. B. Magnusson, T. Naykki, H. Hovind, M. Krysell. *Handbook for Calculation of Measurement Uncertainty*. NORDTEST report TR 537 (project 1589-02) 2003. Internetversion 2003. Can be obtained from www.nordicinnovation.net/nordtest.cfm under link Rapportør: accessed 2007-03-25.
6. Eurachem/CITAC Working Group. *Quantifying Uncertainty in Analytical Measurement*. EURACHEM/CITAC Guide, 2nd Internet edition 2000. www.eurachem.org, accessed 2007-03-25.
7. A. J. Duncan. *Quality control and industrial statistics*. 5th Edition. Homewood. Illinois: Richard D. Irwin, 1986.
8. R. V. Cheeseman & A. L. Wilson (revised by M. J. Gardner). *A manual on analytical quality control for the Water Industry*. Swindon (UK): Water Research Centre; 1989, Publication NS30.
9. ISO 8258. *Shewhart Control Charts*. Geneva: International Organization for Standardization; 1991.
10. ISO/CD 13530:2005. *Water quality Guide to analytical quality control for water analysis*. Geneva: International Organization for Standardization; 2005.
11. R. Caulcutt & R. Boddy. *Statistics for analytical chemists*. New York/London: Chapman & Hall, 1983.
12. W. Funk, V. Dammann, G. Donnevert: Funk W. *Quality assurance in analytical chemistry. Applications in Environmental, Food and Materials Analysis, Biotechnology and Medical Engineering*. 2nd revised Edition. Weinheim: Wiley-VCH, 2006.
13. BIPM, IEC, IFCC, ILAC, ISO, IUPAC, IUPAP, OIML. *International vocabulary of basic and general terms in metrology (VIM)*; Geneva: International Organization for Standardization; 1993.



norden

Nordic Innovation Centre

Return address:

Nordic Innovation Centre,
Stensberggata 25
NO-0170 Oslo, Norway

NORDTEST

NORDTEST is a Nordic Innovation Centre brand offering competence and expertise in the field of harmonizing of norms and methods, a large Nordic net-work of experts, more than 650 recommended Nordic testing methods and 550 published technical reports.

www.nordicinnovation.net

Nordic Innovation Centre

The Nordic Innovation Centre initiates and finances activities that enhance innovation collaboration and develop and maintain a smoothly functioning market in the Nordic region.

The Centre works primarily with small and medium-sized companies (SMEs) in the Nordic countries. Other important partners are those most closely involved with innovation and market surveillance, such as industrial organisations and interest groups, research institutions and public authorities.

The Nordic Innovation Centre is an institution under the Nordic Council of Ministers. Its secretariat is in Oslo.

For more information: www.nordicinnovation.net